

**HORIBA**

Medical

**HORIBA India Private Limited**

246, Okhla Industrial Estate Phase-III,  
New Delhi 110020, India  
Tel : +91 (11) 4646 5000 / 4669 5001  
Fax : +91 (11) 4646 5020  
http : //www.horiba.com  
CIN : U73100DL2006PTC153232

HIN/MED/2023-2024 /10556542  
26<sup>TH</sup> MAY 2023

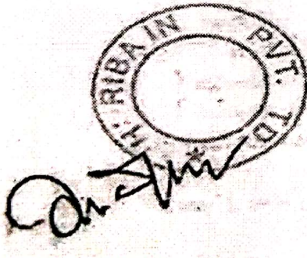
## **CALIBRATION CERTIFICATE**

This is to certify that the Hematology Analyzer Horiba YUMIZEN H550 bearing serial number 204YAXH03729 installed at KRSNAA DIAGNOSTIC LAB MOGA as calibrated on 26<sup>TH</sup> MAY 2023.

Calibrator : ABX MINOCAL  
Lot No. : CX482  
Expiry Date : 05<sup>th</sup> JUNE 2023

The reports of Blank Cycle, Repeatability and Calibration Values were all found in acceptable range.

Next calibration cycle is due on 25<sup>TH</sup> MAY 2024

A circular stamp with the text "HORIBA INDIA PVT. LTD." around the perimeter. In the center of the stamp, there is a handwritten signature in black ink.

Shrish Dixit

(Head- Products & Marketing)  
For Horiba India Pvt. Ltd.

246, Okhla Industrial Estate Phase-  
III, New Delhi 110020, India  
Tel : +91 (11) 4546 5000 / 46695001  
Fax : +91 (11) 4646 5020  
http : //www.horiba.com  
CIN : U73100DL2006PTC1M232



Calibration

Calibrator Information

Sample ID: **CX183** Name: **MINOCAL** Exp. date: **05/07/2023**  
 Lot number: **CX183** Modified on:

Coefficients	WBC	RBC	HGB	HCT	PLT	MPV
	New	1.158	0.940	1.008	1.036	0.996
Current	1.158	0.945	1.030	1.010	0.900	1.019
Target	8.90	4.52	12.8	37.1	258	10.3
Mean	8.57	4.57	12.7	36.0	250	10.2
CV(%)	1.36	0.50	0.54	0.72	3.67	1.02

Selected runs (5 minimum) **6/5**

Run Date & Time	WBC (10 <sup>3</sup> /μL)	RBC (10 <sup>6</sup> /μL)	HGB (g/dL)	HCT (%)	PLT (10 <sup>3</sup> /μL)	MPV (fL)
26/05/2023 02:21:56 PM	8.64	4.59	12.8	36.1	246	10.1
26/05/2023 02:23:29 PM	8.66	4.58	12.8	36.0	253	10.2
26/05/2023 02:25:01 PM	8.59	4.59	12.8	36.3	243	10.0
26/05/2023 02:26:37 PM	8.44	4.54	12.6	35.6	263	10.3
26/05/2023 02:28:06 PM	8.69	4.54	12.7	35.8	239	10.2
26/05/2023 02:29:33 PM	8.42	4.56	12.8	36.0	259	10.2

QUAL COMM REAG SYST

v12.1.4 technician

READY

24/01/2024 03:59 PM

*Handwritten signature*