

CALIBRATION CERTIFICATE

Name of the customer	TAPADIA DIAGNOSTIC CENTRE ADD BANSILAL NAGAR,STATION ROAD,CHHATRAPATI SAMBHAJINAGAR(AURANGABAD)-431005 CONT NO.(0240)2354558,9158324242
----------------------	--


Make:	HORIBA MEDICAL FRANCE
Product Name:	ABX PENTRA C 200
S.No.	1906C20162D

This is to certify that the ABX PENTRA C200 Fully automated clinical Biochemistry analyzer has been duly inspected and calibrated on 20-05-2023. The instrument is working satisfactorily and the next calibration due on 19-05-2024.

S.No.	Test Parameters	Measured	Remarks			
1	Input Voltage (230±10V)	228	Pass			
2	UPS (2KVA)	1.0 KVA	Pass			
3	Input Frequency (50-60Hz)	50 Hz	Pass			
4	Operating Temp. (20-25 Deg c.)	25 Deg. C	Pass			
5	Software Version	1002	Pass			
6	Precision test (CV≤2%) Appendix 1	0.4	Pass			
7	Spectro gains (2to10) Appendix 2					
	Wavelength					
	a)340nm	9.07	Pass	e)570nm	9.11	Pass
	b)405nm	8.94	Pass	f)600nm	8.89	Pass
	c)510nm	9.02	Pass	g)660nm	8.99	Pass
	d)546nm	8.98	Pass	h)700nm	8.76	Pass

Appendix -1

Appendix -2

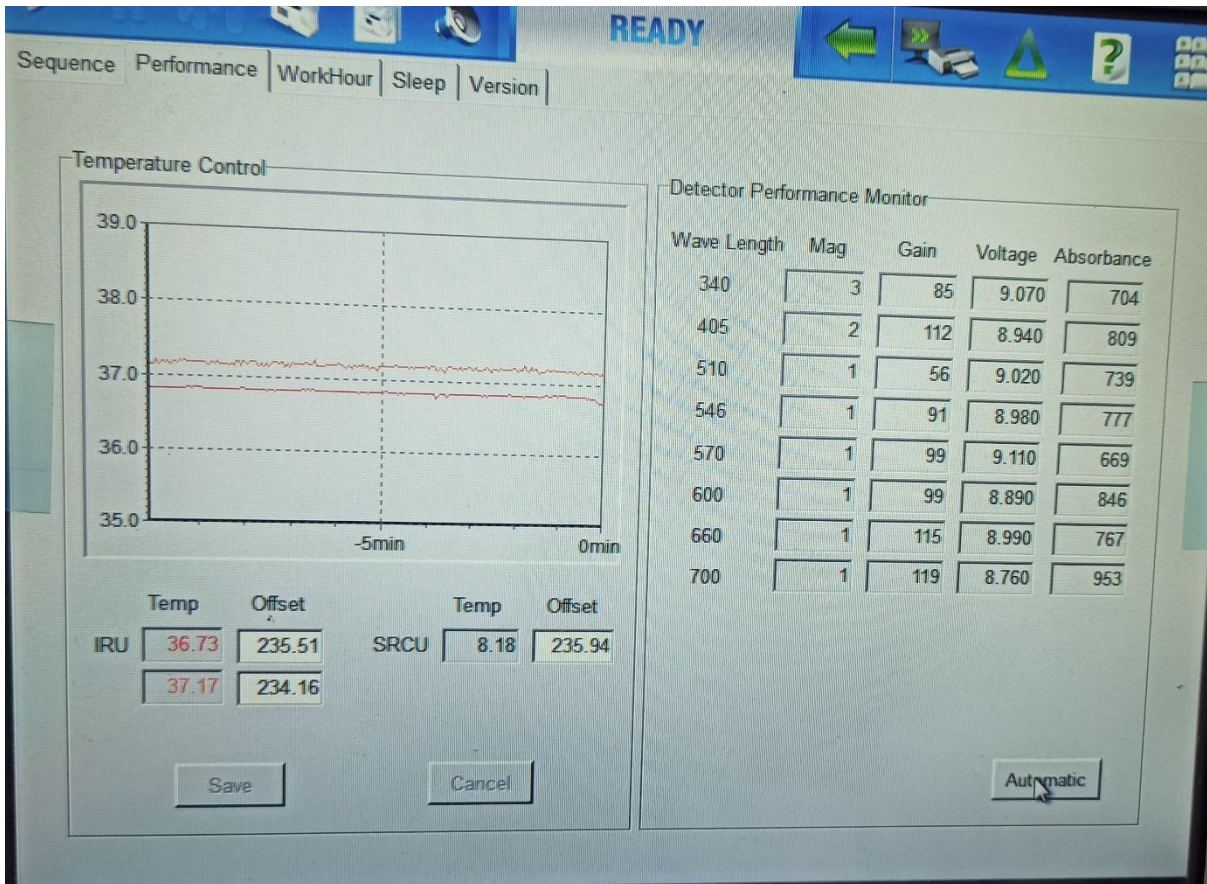

Note: Refer Page No 385 in the User manual, for the Spectro Gain

For HORIBA INDIA PVT. LTD.

Ananta Landge
(SENIOR ENGINEER)
CLINICAL CHEMISTRY