

INSTALLATION
QUALIFICATION

For

TRANSASIA
ERBA ELITE 580
AUTOMATED HEAMATOLOGY ANALYZER

DR. B.LAL CLINICAL LABORATORY PVT. LTD

Manufactured by ERBA MANNHEIM
&

Marketed by:
Transasia Bio-Medicals Ltd.,
Transasia House,
Chandivali Studio road,
Andheri (E),
MUMBAI - 400 072



Table of Contents

Sr. No.	Contents	Page No.
I	Approval of the IQ procedure	
II	Instructions	
III	Scope	
IV	Ancillary Information	
V	Installation Qualification	
VI	Installation Procedure	
VII	Comments	
VIII	System Certification	
IX	Appendices	
	i	Installation Report Dt. _____
	ii	ISO 9002 certificate
	iii	Sample Page of the Logbook



I. Approval of the IQ procedure:

DR. B LAL CLINICAL LABORATORY PVT. LTD, HEMATOLOGY Laboratory and Transasia are jointly responsible for the installation of the system ERBA HEMATOLOGY Analyzer, Model: ELITE 580, Serial No. K11051912060 in the clinical lab of JAIPUR NATIONAL UNIVERSITY as per the attached protocol.

Protocol Performed By: Transasia Representative

Name : ICHCHESH DESHWAL
Title : INSTALLATION QUALIFICATION
Company : TRANSASIA BIO-MEDICALS LTD.

Ichchesh Deshwal
Signature:
10/06/2020

Date:

Validation Team from _____;

Name : ANKUSH JAIN
Designation : APPLICATION SPECIALIST
Department : TSD

Customer Authorizations:

Name : MR. AMIT SHARMA
Title : INSTALLATION QUALIFICATION
Site : SJAR

Signature: *Amit Sharma*

Date: 10/06/2020



II. Instructions

1. This document is to be completed at the time the system is shifted to its current location (new) and set up for operation.
2. An authorized TRANSASIA representative will check the system and enter the specific data as outlined in the appropriate Installation Qualification. Each result will be noted and dated.
3. Employee of DR B LAL CLINICAL LABOATORY PVT LTD will verify each result and sign in the last page. The members of the validation team will carry this out.
4. ALL deviations from normal specification to include any problems with installation will be noted under COMMENTS. All resolution to such problems will also be noted in the COMMENTS section. Additional space is provided at the end of this protocol for the same.
5. This document contains proprietary information and is in no way to be copied, photographed or duplicated in any way without expressed written authorization by the Transasia Bio-Medicals Ltd., Transasia House, Mumbai.

Validation Team :

Name: ICHCHESH DESHWAL

Designation: SERVICE ENGINEER

Signature:

Ichchesh Deshwali
10/01/20

Date:



III. Scope

This Installation Qualification protocol will be performed on the ERBA Hematology Analyzer, Model ELITE 580, Serial No. K11051912060 located in DR B LAL LAB CLINICAL LABORATORY HEMATOLOGY LAB This Protocol will define the documentation that will be used to evaluate the instruments installation in accordance with the manufacture's specifications and intended use. Successful completion of this protocol will verify that the instrument identified has been installed in accordance with the intended usage.

Installation checks will also be performed to verify that the instrument has been installed with proper connections and utilities.

Trained, knowledgeable personnel will perform qualification studies.

Any exceptional conditions encountered during the qualification studies will be identified for review. Exceptional conditions will be investigated and the appropriate course of action determined. All documents will be initialed and dated.

Validation Team:

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Ichchesh Deshwale
10/01/20

Date:



IV. Ancillary Information.

a. Certification of Purchase Order Compliance

I certify to the best of my knowledge, the instrument is purchased under Purchase order No. _____, Dt. _____ sent against Quotation number _____ dt. _____ is in compliance with the specifications of the Purchase order.

Verified By : _____

Date : _____



b. Utilities

Sr.No.	Utility	Yes / No	Verified By	Date
1.	Environmental condition as per requirement: (Ambient range of temperature 15 - 30 °C, relative humidity 30% to 85%, air conditioning facility, non exposure to direct sunlight, non-interference from high frequency radio waves)	Yes / No		
2.	Adequate space for installation : (Minimum in mm. W 600 X D 600 X H 552 for the main unit clearance of around 50 cm from back around 50cm on top and around 50 cm on sides for the main unit)	Yes / No	<i>Kalshreshna</i>	10/6/20
3.	DIL-ELITE 580; LYSE1, LYSE2 & LYSE 3 BOTTLES to be placed within a distance of 2 meters :	Yes / No		
4.	Power Source Requirements* It should have minimum five Samps plug. It should have proper grounding. In case of online UPS minimum power handling capacity should be minimum 1KVA Line- Neutral voltage: <u>230</u> Line -Earth voltage: <u>3vlt</u> Neutral-Earth voltage: <u>22*</u>	Yes / No		

* Encircle applicable source

Validation Team :

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Kalshreshna
10/6/20

Date:



c. The instrument has been verified for the following

Sr.No.	Verification	Yes / No	Verified By	Date
1.	Instrument is identified	Yes / No		
2.	Manufacturer's specifications are included	Yes / No		
3.	Accessories / Consumables are listed	Yes / No	<i>I. Deshwal</i>	10/6/20
4.	Manufacturer's certificate of Compliance attached	Yes / No		

Validation Team :

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

I. Deshwal
10/6/20

Date:



V. Installation Qualification

A. Equipment Description

This ERBA ELITE 580 is a fully automated five part Hematology analyzer for in vitro diagnostic use in clinical laboratories. The instrument provides accurate and precise test results for (29) parameters including three histograms & one scatter- grams.

Instrument identification		Verified by	Date
Equipment Name	Automated Hematology		
Model	ELITE 580		
Manufacturer	Erba Mannheim		
Marketed By	Transasia		
Equipment #			
Serial Number	K11051912060		
Size (in mm)	W 600 X D 600 X H 552		
Power	AC 220 V		
Frequency	50 - 60 Hz		
Power Consumption	Less Than 250 VA		

Validation Team:

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Date:



Ichchesh Deshwali
10/6/20

Installation Qualification

Consumables such as H-Clean, DII, ELITE 580, LYSE1 & LYSE2 were supplied along with instrument.

Currently a sufficient stock of the same is being maintained Yes No

C. List of Manuals, Certificates and Drawings

Transasia provides the following with the instrument.

1. Instructions For use
2. User's Guide

D. Change Control Procedure

The instrument will not be altered, enhanced, modified or substituted for another system until a formal Change Control Authorization is approved from Transasia Bio-Medicals Ltd. and DR B LAL CLINICAL LABORATORY ALWAR .

E. Maintenance

The instrument listed within this document will be placed under the control of the purchasing institution with respect to proper maintenance procedures as detailed in the User Manual.

A trained analyst using the manuals provided with the instrumentation can perform simple maintenance. Upon expiration of the warranty period Transasia offers several levels of Maintenance Agreements and Performance Testing services to assist you in maintaining GLP/GMP compliance. Contacting your local representative and requesting the additional Service Agreement can supply additional information.

Validation Team :

Name: ICHCHESH DESHWAL
Designation: AREA SERVICE MANAGER
Signature: *Ichchesh*
Date: 10/6/20



F. Spare Parts

Transasia strongly recommends the end user maintain a basic of consumable parts onsite to minimize down time due to minor failures. They have provided a list of such consumable parts and the same is also available in the Operator's Manual.

C. Equipment Logs

Title	Location	Verified by	Date

Sample page of the logbook is attached to this document

Effective date:

Validation Team :

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Ichchesh
10/6/20

Date:



H. Installation Procedure

(These had been performed at the time of original installation at the initial location)

1. Unpacking Checklist

Refer to Page-13 of ERBA ELITE 580 Instruction For Use

2. Check Before Installation

Refer to Page-13 of ERBA ELITE 580 Instruction For Use

3. Grounding

Refer to Page-13 of ERBA ELITE 580 Instruction For Use

4. Installation Environment & Space

Refer to Page-13 of ERBA ELITE 580 Instruction For Use

Validation Team:

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Ichchesh
10/6/20

Date:



COMMENTS:

NO DEVIATION FOUND EVERYTHING FOUND SATISFACTORY

Validation Team :

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Ichchesh
10/06/20

Date:



VII. System Certification

Study data has determined that the system described in this document either meets all criteria outlined in this independently Installation Qualification Protocol, or exceptional conditions have been identified and documentation included. Exceptional conditions, if any, have been addressed. The system is ready for specified usage.

Report Performed By : Transasia Representative

Name : ICHCHESH DESHWAL

Title : INSTALLATION QUALIFICATION Signature :

Company: TRANSASIA BIO-MEDICALS LTD. Date :

ICHCHESH DESHWAL
10/6/20

Customer Authorizations:

Name : MR. MOHAR SINGH

Title : INSTALLATION QUALIFICATION Signature:

Company : Date :

Name : MR. AMIT SHARMA

Title : INSTALLATION QUALIFICATION Signature:

Company: *g.R. B. Lal Clinical Lab. Pvt. Ltd.* Date : 10/6/20

Amn



Date: 10-6-2020

Reagent Check done

Printer checked

Analyzer switched ON at

SELF CHECK performed

RINSE CYCLE completed

Background limits within acceptable range

Analysis start time

Analysis end time

No. of samples analyzed

Shut down procedure done

Analyzer switched OFF at

Recorded by:

Checked by:

Jeddyump

[Signature]



Date: 10/6/20

ERBA- ELIE 580
AUTOMATED HEMATOLOGY ANALYZER

PERFORMANCE
QUALIFICATION

For

“ DR B LAL CLINICAL LABORATORY PVT LTD ”

Marketed by:
Transasia Bio-Medicals Ltd.,
(ISO 9002 CERTIFIED)
Transasia House,
Chandivali Studio road,
Andheri (E),
MUMBAI - 400 072



Table of Contents:

Sr. No.	Contents	Page No.
I	Approval of the PQ procedure	3
II	Instructions	4
III	Scope	5
IV	Performance Qualification	6
V	System Certification	10



I. Approval of the PO procedure

Both DR B LAL CLINICAL LABORATORY PVT LTD and Transasia are jointly responsible for conducting the Performance Check of the Hematology Analyzer, Model : ERBA - ELIE 580, Serial No. K11051912060 in the clinical lab of DR B LAL CLINICAL LABORATORY PVT LTD as per the attached protocol.

Protocol Performed By: Transasia Representative

Name : ANKUSH JAIN
Title : PERFORMANCE QUALIFICATION
Company : TRANSASIA BIO-MEDICALS LTD.

Signature: *ANKUSH JAIN*
Date: 10-6-2020

Validation Team from :

Name : ANKUSH JAIN
Designation : APPLICATION SUPPORT
Department : TSD

ANKUSH JAIN

Name : ICHCHESH DESHWAL
Designation : SERVICE ENGINEER
Department : TSD

Customer Authorizations:

Name : MR. MOHAR SINGH
Title : PERFORMANCE QUALIFICATION
Site :

Signature: *MOHAR SINGH*
Date: 10/6/20



II. Instructions

1. An authorized TRANSASIA representative will check for the performance of the instrument and enter the specific data as outlined in the Performance Qualification. Each result will be noted and dated.
2. Performance checks on a regular basis described in the Further Performance Checks (vide-infra) will be responsibility of the customer's personnel.
3. Employee of DR B LAL CLINICAL LABORATORY PVT LTD will verify each result and sign in the last page. The members of the validation team will carry this out.
4. ALL deviations from the acceptance criteria detailed in this document will be noted in the COMMENTS section at the end of each IQ protocol. All resolution to such problems will also be noted in the COMMENTS section, and must be resolved prior to issuance of a SYSTEM CERTIFICATION. These will be an additional cost to the purchasing institution (CUSTOMER). However this additional cost will be waived when this test is conducted at time of initial performance check of new instruments.
5. Any test data that does not meet the specified acceptance criteria will be submitted to the appropriate laboratory personnel for solution. All steps taken subsequently will be documented.
6. This document contains proprietary information and is in no way to be copied, photographed or duplicated in any way without expressed written authorization by the Production Manager at Transasia Bio-Medicals Ltd., Transasia House, Mumbai.

Validation Team:

Name ANKUSH JAIN
Designation APPLICATION SPECIALIST
Signature 
Date 10-6-2020




III. Scope

This Performance Qualification protocol will be performed on the Hematology Analyzer, Model ERBA - ELIE 580, Serial NO K11051912060 located in **DR B LAL CLINICAL LABORATORY PVT LTD.** This Protocol will define the documentation that will be used to evaluate the instruments installation in accordance with the manufacture's specifications and intended use. Successful completion of this protocol will verify that the instrument identified is performing in accordance with the intended usage.

Trained, knowledgeable personnel will perform qualification studies.

Any exceptional conditions encountered during the qualification studies will be identified for review. Exceptional conditions will be investigated and the appropriate course of action determined. All documents will be initialed and dated.

Validation Team:

Name	ANKUSH JAIN
Designation	APPLICATION SPECIALIST
Signature	
Date	10-6-2020



IV. Performance Qualification

a. Instrument Identification

Verified Date

1. Model Name ERBA – ELIE 580 10-6-2020
2. Serial Number K11051912060

b. Following is a list of tests to be performed and verified:

<u>Test No.</u>	<u>Test Name</u>	<u>Test Purpose</u>	<u>Verified Date</u>
02	Sample Processing	Ability to process samples	
03	Further Performance Checks	Regular Maintenance	10-6-2020



Validation Team:

Name ANKUSH JAIN
Designation APPLICATION SPECIALIST
Signature *Ankush Jain*
Date *10-6-2020*

c. Performance Testing

Test 1

Test Name: Sample Processing
Purpose: Ability to Process Samples
Method:

1. Run the control samples five times consecutively

Acceptance Criteria: Each of the results obtained above should be within the range as specified in the control chart.

Parameters Values for Verification:

RBC Count:

Test	Control Values	Results Obtained	Pass	Fail
1.	4.35 - 4.83	4.61	PASS	
2.	4.35 - 4.83	4.64	PASS	
3.	4.35 - 4.83	4.65	PASS	
4.	4.35 - 4.83	4.69	PASS	
5.	4.35 - 4.83	4.62	PASS	

Validation Team:

Name ANKUSH JAIN
Designation APPLICATION SPECIALIST
Signature *Ankush Jain*
Date 10-6-2020



WBC Count:

Test	Control Values	Results Obtained	Pass	Fail
1.	6.78 - 8.78	7.84	PASS	
2.	6.78 - 8.78	7.75	PASS	
3.	6.78 - 8.78	7.84	PASS	
4.	6.78 - 8.78	7.72	PASS	
5.	6.78 - 8.78	8.08	PASS	

Hemoglobin:

Test	Control Values	Results Obtained	Pass	Fail
1.	12.8 - 14.0	13.5	PASS	
2.	12.8 - 14.0	13.3	PASS	
3.	12.8 - 14.0	13.5	PASS	
4.	12.8 - 14.0	13.5	PASS	
5.	12.8 - 14.0	13.4	PASS	

HCT:

Test	Control Values	Results Obtained	Pass	Fail
1.	39.6 - 45.24	42.5	PASS	
2.	39.6 - 45.24	42.7	PASS	
3.	39.6 - 45.24	42.6	PASS	
4.	39.6 - 45.24	43.0	PASS	
5.	39.6 - 45.24	42.4	PASS	

Platelet Count:

Test	Control Values	Results Obtained	Pass	Fail
1.	202 - 282	250	PASS	
2.	202 - 282	253	PASS	
3.	202 - 282	247	PASS	
4.	202 - 282	241	PASS	
5.	202 - 282	251	PASS	

Validation Team:

Name ANKUSH JAIN
 Designation APPLICATION SPECIALIST
 Signature *ANKUSH*
 Date 10-6-2020



Test 2

Test Name:

1. Tests for checking the performance of the instruments during analysis
2. Tests for checking long term performance of the instrument

Purpose:

The purpose of the above checks is to ensure the reliability of the results being obtained.

Method:

1. During Sample analysis:

To run control samples each time the instrument is used for sample analysis and verification of the results of the controls to be within the reference range to be established by performance of the precision experiments.

2. Long term Performance

This is to be checked by Levy Jennings plots to be updated once in six months

Validation Team:

Name ANKUSH JAIN
Designation APPLICATION SPECIALIST
Signature *Ankush Jain*
Date *10-6-2020*



V. System Certification

Study data has determined that the system described in this document either meets all criteria outlined in this Performance Qualification Protocol, or exceptional conditions have been identified and documentation included. Exceptional conditions, if any, have been addressed. The system is ready for specified usage.

Report Performed By: Transasia Representative

Name : ANKUSH JAIN

Title : PERFORMANCE QUALIFICATION Signature:

Company: TRANSASIA BIO-MEDICALS LTD. Date :

Handwritten signature
10-6-2020

Customer Authorizations:

Name : MR. MOHAR SINGH

Title : PERFORMANCE QUALIFICATION Signature:

Site : DR B LAL LAB ALWAR

Date :

Name :MR. AMIT SHARMA

Title : PERFORMANCE QUALIFICATION Signature:

Site : DR B LAL LAB, ALWAR SIKAR

Date 10-6-2020





L-J QC Table

Editor: admin
 Existing / Total: 5/500
 QC Sample ID:

QC Mode: Whole Blood-CBC+DIFF
 Level: Normal

File No.: 2
 Date Range: 2020/06/10-2020/06/10
 Exp. Date: 2020/07/10

Lot No.: EH2005N
 Print Time: 2020/06/10 08:50:24

	Date	Time	Operator	WBC	Neu%	Lymph	Mon%	Co%	Bas%	Hgb	Hct	Hemc	MCV	MCH	MCHC	RDW	CRP	SD	PLT	MPV	POR	SDPW	CV	PCT	P-LCR	P-LCC			
TARGET	1	7	1	136	26.7	29.7	7.1	5.9	52.1	4.45	2.22	3.6	0.47	5.65	4.5	13.3	41	86.1	20	32.5	36.1	52.1	245	15.5	12.7	16	0.248	263	69
LEMSON	1	7	1	1	0	0	0	5.9	6	3.7	6.7	3.5	0.47	3.1	6.24	0.6	2	5	2.5	5	3	35	40	3	5	3	0.1	3	25
1	2020/06/10	06:34:22	admin	7.84	53.0	30.0	7.3	3.7	73.1	4.85	2.55	3.57	0.25	5.74	4.51	13.5	42.8	92.1	25.8	31.4	36.2	52.2	280	9.9			0.248	263	60
2	2020/06/10	06:43:44	admin	7.75	53.7	26.7	3.1	3.5	71.4	4.85	2.22	3.63	0.27	5.84	4.54	13.5	42.7	91.5	29.5	31.6	36.2	52.3	280	11.0			0.264	266	67
3	2020/06/10	06:45:05	admin	7.34	53.0	30.1	7.6	3.5	72.8	4.81	2.55	3.63	0.27	5.70	4.58	13.4	42.8	91.7	26.8	31.6	36.2	52.1	241	9.2			0.245	252	62
4	2020/06/10	06:46:26	admin	7.72	53.2	26.5	3.2	3.1	72.3	4.87	2.28	3.63	0.24	5.89	4.68	13.6	43.2	91.7	26.8	31.4	36.2	52.3	241	10.3			0.248	270	67
5	2020/06/10	06:47:31	admin	8.08	57.0	30.3	3.4	3.7	72.7	4.86	2.43	3.63	0.26	5.87	4.62	13.5	42.4	91.9	29.2	31.6	36.2	51.7	251	10.1			0.250	258	67

Handwritten signature

OPERATIONAL
QUALIFICATION

For

TRANSASIA

ELITE 580

AUTOMATED HEMATOLOGY ANALYZER

DR. B LAL CLINICAL LABORATORY PVT LTD

Marketed by:
Transasia Bio-Medicals Ltd.,
(ISO 13485 CERTIFIED)
Transasia House,
Chandivali Studio road,
Andheri (E),
MUMBAI - 400 072



Table of Contents

Sr. No.	Contents	Page No.
I	Approval of the OQ procedure	
II	Instructions	
III	Scope	
IV	Operational Qualification	
V	System Certification	



I. Approval of the OQ procedure:

DR B LAL CLINICAL LABORATORY PVT LTD and Transasia are jointly responsible for operational check of the HEMATOLOGY Analyzer, Model: ELITE 580, serial no. K11051912060 in the clinical lab of DR B LAL CLINICAL LABORATORY PVT LTD as per protocol attached.

Protocol Performed by: Transasia Representative

Name : ICHCHESH DESHWAL
Title : OPERATIONAL QUALIFICATION
Company : TRANSASIA BIO-MEDICALS LTD.

Signature :
Date :

Ichchesh
10/06/20

Validation Team from _____

Name : ICHCHESH DESHWAL
Designation : APPLICATION SPECIALIST
Department : TSD

Customer Authorization:

Name : MR. MOHAR SINGH
Title : OPERATIONAL QUALIFICATION
Site : DR B LAL CLINICAL LABORATORY PVT. LTD.

Signature : *Mohar Singh*
Date : *10/6/2020*



II. Instructions

1. The TRANSASIA representative will check each module and enter the specific data as described in the Operational Qualification. Each result will be noted and dated.
2. Employee of DR B LAL LABORATORY PVT LTD will verify each result and sign in the last page. The member/s of the validation team will be responsible for the same.
3. Any deviations from the acceptance criteria detailed in this document will be noted in the COMMENTS section of the OQ protocol. All resolution to such problems will also be noted in the COMMENTS section, and must be resolved prior to issuance of a SYSTEM CERTIFICATION. This will be an additional cost to the purchasing institution (CUSTOMER). However this additional cost will be waived when this test is conducted at time of initial performance check of new instruments.
4. Any test data, which does not meet the specified acceptance criteria, will be submitted to the appropriate laboratory personnel for solution. All steps taken subsequently will be documented.
5. This document contains proprietary information and is in no way to be copied, photographed or duplicated in any way without expressed written authorization by the Product Manager at Transasia Bio-Medicals Ltd., Transasia House, Mumbai.

Validation Team:

Name: ICHCHESH DEAHWAL

Designation: AREA SERVICE MANAGER

Signature:

Ichchesh Deahwal
10/10/20

Date:



III. Scope

This Operational Qualification protocol will be performed on the Hematology Analyzer, Model ELITE 580, Serial No. K11051912060 located in DR B LAL CLINICAL LABORATORY PVT LTD. in Clinical laboratory of DR B LAL CLINICAL LABORATORY PVT LTD ALWAR RAJASTHAN. This Protocol will define the documentation that will be used to evaluate the instruments installation in accordance with the manufacturer's specifications and intended use. Successful completion of this protocol will verify that the instrument identified is performing in accordance with the intended usage.

Trained, knowledgeable personnel will perform qualification studies.

Any exceptional conditions encountered during the qualification studies will be identified for review. Exceptional conditions will be investigated and the appropriate course of action determined. All documents will be initialed and dated.

Validation Team:

Name: ICHCHESH DESHWAL
Designation: AREA SERVICE MANAGER
Signature: *Ichchesh Deshwali*
Date: 10/11/20



COMMENTS:
NO DEVIATION FOUND

Validation Team :

Name: ICHCHESH DESHWAL

Designation: AREA SERVICE MANAGER

Signature:

Ichchesh
10/6/20

Date:



VII. System Certification

Study data has determined that the system described in this document either meets all criteria outlined in this Operational Qualification Protocol, or exceptional conditions have been identified and documentation included. Exceptional conditions, if any, have been addressed. The system is ready for specified usage.

Report Performed By : Transasia Representative

Name : ICHCHESH DESHWAL

Title : OPERATIONAL QUALIFICATION Signature : *Ichchesh*
11/6/20

Company : TRANSASIA BIO-MEDICALS LTD. Date :

Customer Authorizations:

Name : MR. MOHAR SINGH

Title : OPERATIONAL QUALIFICATION Signature : *Mohar Singh*

Company : DR B LAL LAB ~~ALWAR~~ SIRAR Date : 10/6/20



INSTITUTE NAME

DR B LAL CLINICAL LABORATORY

Instrument Serial Number: K11051912060

Carryover Study

Date performed:

Carryover calculation:

$$\text{Carryover \%} = (L1-L3) / (H3-L3) * 100.$$

Interpretation of results :

- 1) If (L1-L3) is equal to a negative number or zero then stop as there is no evidence of carryover.
- 2) The percentage carryover effect should be less than the imprecision of the assay listed by manufacturer.

Analytes					
Instrument	WBC	RBC	Plt	Hb	Hct
H1	6.46	5.2	325	13.3	39.8
H2	6.29	5.18	326	13.3	39.6
H3	6.26	5.15	307	13.3	39.4
L1	0	0	3	0	0
L2	0	0	0	0	0
L3	0	0	0	0	0
% age Carryover	0.00	0.00	0.98	0.00	0.00

Company Signature

Sig:

Date:



Customer Authorization

Sig:

Date:

Sushil
10/6/20

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: H1
Run Time: 2020/06/10 07:58
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	6.46	4.00-10.00	10 ³ /uL				
2 RBC	5.20	3.50-5.50	10 ⁶ /uL				
3 HGB	13.3	11.0-16.0	g/dL				
4 HCT	39.8	37.0-54.0	%				
5 MCV	76.5 ↓	80.0-100.0	fL				
6 MCH	25.6 ↓	27.0-34.0	pg				
7 MCHC	33.4	32.0-36.0	g/dL				
8 RDW-CV	14.8	11.0-16.0	%				
9 RDW-SD	40.6	35.0-56.0	fL				
10 PLT	325 ↑	100-300	10 ³ /uL				
11 MPV	11.4	6.5-12.0	fL				
12 PCT	0.372 ↑	0.108-0.282	%				
13 P-LCR	35.8	11.0-45.0	%				
14 P-LCC	116 ↑	30-90	10 ⁹ /L				

Sample Type:
Description:

Microscopic exam. Time:



Submitter:

Operator: admin

Approver: admin

Sampling Time: 2020/06/10 07:58

Delivery Time: 2020/06/10 07:58

Validated Time: 2020/06/10 08:10

Report Time: 2020/06/10 08:10

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: H2
Run Time: 2020/06/10 08:01
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	6.29	4.00-10.00	10 ³ /uL				
2 RBC	5.18	3.50-5.50	10 ⁶ /uL				
3 HGB	13.3	11.0-16.0	g/dL				
4 HCT	39.6	37.0-54.0	%				
5 MCV	76.5 ↓	80.0-100.0	fL				
6 MCH	25.6 ↓	27.0-34.0	pg				
7 MCHC	33.5	32.0-36.0	g/dL				
8 RDW-CV	15.0	11.0-16.0	%				
9 RDW-SD	41.1	35.0-56.0	fL				
10 PLT	326 ↑	100-300	10 ³ /uL				
11 MPV	11.5	6.5-12.0	fL				
12 PCT	0.377 ↑	0.108-0.282	%				
13 P-LCR	36.1	11.0-45.0	%				
14 P-LCC	118 ↑	30-90	10 ⁹ /L				

Sample Type:
Description:

Microscopic exam. Time:

ATMC

Submitter:

Operator: admin

Approver: admin

Sampling Time: 2020/06/10 08:01

Delivery Time: 2020/06/10 08:01

Validated Time: 2020/06/10 08:10

Report Time: 2020/06/10 08:10

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: H3
Run Time: 2020/06/10 08:03
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	6.26	4.00-10.00	10 ³ /uL				
2 RBC	5.15	3.50-5.50	10 ⁶ /uL				
3 HGB	13.3	11.0-16.0	g/dL				
4 HCT	39.4	37.0-54.0	%				
5 MCV	76.5 ↓	80.0-100.0	fL				
6 MCH	25.8 ↓	27.0-34.0	pg				
7 MCHC	33.6	32.0-36.0	g/dL				
8 RDW-CV	14.6	11.0-16.0	%				
9 RDW-SD	40.0	35.0-56.0	fL				
10 PLT	307 ↑	100-300	10 ³ /uL				
11 MPV	11.4	6.5-12.0	fL				
12 PCT	0.352 ↑	0.108-0.282	%				
13 P-LCR	36.1	11.0-45.0	%				
14 P-LCC	111 ↑	30-90	10 ⁹ /L				

Sample Type:
Description:

Microscopic exam. Time:

Submitter:
Sampling Time: 2020/06/10 08:03
Report Time: 2020/06/10 08:06

Operator: admin
Delivery Time: 2020/06/10 08:03
Remarks:

Approver: admin
Validated Time: 2020/06/10 08:06

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: L1
Run Time: 2020/06/10 08:00
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	0.00 ↓	4.00-10.00	10 ³ /uL				
2 RBC	0.00 ↓	3.50-5.50	10 ⁶ /uL				
3 HGB	0.0 ↓	11.0-16.0	g/dL				
4 HCT	0.0 ↓	37.0-54.0	%				
5 MCV	***	80.0-100.0	fL				
6 MCH	***	27.0-34.0	pg				
7 MCHC	***	32.0-36.0	g/dL				
8 RDW-CV	**	11.0-16.0	%				
9 RDW-SD	***	35.0-56.0	fL				
10 PLT	0 ↓	100-300	10 ³ /uL				
11 MPV	**	6.5-12.0	fL				
12 PCT	***	0.108-0.282	%				
13 P-LCR	**	11.0-45.0	%				
14 P-LCC	****	30-90	10 ⁹ /L				

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: admin

Sampling Time: 2020/06/10 08:00

Delivery Time: 2020/06/10 08:00

Validated Time: 2020/06/10 08:10

Report Time: 2020/06/10 08:10

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: L3
Run Time: 2020/06/10 08:05
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	0.00 ↓	4.00-10.00	10 ³ /uL				
2 RBC	0.00 ↓	3.50-5.50	10 ⁶ /uL				
3 HGB	0.0 ↓	11.0-16.0	g/dL				
4 HCT	0.0 ↓	37.0-54.0	%				
5 MCV	***	80.0-100.0	fL				
6 MCH	***	27.0-34.0	pg				
7 MCHC	***	32.0-36.0	g/dL				
8 RDW-CV	**	11.0-16.0	%				
9 RDW-SD	***	35.0-66.0	fL				
10 PLT	0 ↓	100-300	10 ³ /uL				
11 MPV	**	6.5-12.0	fL				
12 PCT	***	0.108-0.282	%				
13 P-LCR	**	11.0-45.0	%				
14 P-LCC	****	30-90	10 ⁹ /L				

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: admin

Sampling Time: 2020/06/10 08:05

Delivery Time: 2020/06/10 08:05

Validated Time: 2020/06/10 08:10

Report Time: 2020/06/10 08:10

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:

Sample Type:

Sample ID: L2

Last Name:

Department:

Run Time: 2020/06/10 08:02

Gender:

Patient ID:

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	0.00 ↓	4.00-10.00	10 ³ /uL				
2 RBC	0.00 ↓	3.50-5.50	10 ⁶ /uL				
3 HGB	0.0 ↓	11.0-16.0	g/dL				
4 HCT	0.0 ↓	37.0-54.0	%				
5 MCV	***	80.0-100.0	fL				
6 MCH	***	27.0-34.0	pg				
7 MCHC	***	32.0-36.0	g/dL				
8 RDW-CV	**	11.0-16.0	%				
9 RDW-SD	***	35.0-56.0	fL				
10 PLT	0 ↓	100-300	10 ³ /uL				
11 MPV	**	6.5-12.0	fL				
12 PCT	***	0.108-0.282	%				
13 P-LCR	**	11.0-45.0	%				
14 P-LCC	****	30-90	10 ⁹ /L				

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver: admin

Sampling Time: 2020/06/10 08:02

Delivery Time: 2020/06/10 08:02

Validated Time: 2020/06/10 08:06

Report Time: 2020/06/10 08:06

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

Hematology Analysis Report

First Name:

Sample Type:

Sample ID: background

Last Name:

Department:

Run Time: 2020/06/10 05:05

Gender:

Patient ID:

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	0.01	↓	10 ³ /uL				
2 RBC	0.00	↓	10 ⁶ /uL				
3 HGB	0.0	↓	g/dL				
4 HCT	0.0	↓	%				
5 MCV	***		fL				
6 MCH	***		pg				
7 MCHC	***		g/dL				
8 RDW-CV	**		%				
9 RDW-SD	***		fL				
10 PLT	0	↓	10 ³ /uL				
11 MPV	**		fL				
12 PCT	***		%				
13 P-LCR	**		%				
14 P-LCC	****		10 ⁹ /L				

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver:

Sampling Time: 2020/06/10 05:05

Delivery Time: 2020/06/10 05:05

Validated Time:

Report Time: 2020/06/10 07:54

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

INSTITUTE NAME


DR BLAL CLINICAL LABORATORY

Instrument Serial Number: _____ K11051912060

Inter Instrument Comparison-PLT

Date performed:

SID NO.	X8	ELITE 580	% BIAS
85001330	320	331	-0.6
85001329	321	324	-0.9
85001328	319	336	-5.1
85001323	378	385	-2.3
85001321	283	304	-6.9
85001318	419	411	1.9
85001316	154	163	-5.5
85001315	534	530	0.8
85001313	451	468	-3.8
85001310	86	81	6.2
85001309	383	391	-2.0
85001306	318	337	-5.8
85001304	165	172	-4.1
9600205	183	184	-0.5
9600206	152	148	4.1
85001303	122	128	-4.7
85001317	314	308	2.8
85001300	115	112	2.7

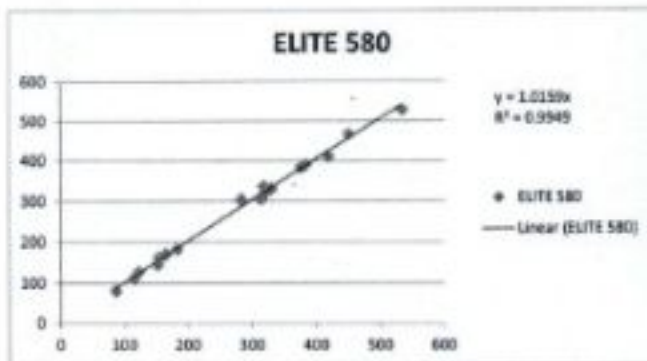

Company Representative

Sig: _____

Date: _____



Customer Authorization

Sig: _____

Date: _____

10/6/20

INSTITUTE NAME

DR B LAL CLINICAL LABORATORY


Instrument Serial Number: _____

K1105191200

Inter Instrument Comparison-HCT

Data performed:

BID NO.	X _B	ELITE 580	% BIAS
85001320	36.7	36.7	0.0
85001329	39.8	39.9	-0.3
85001325	33.8	34.3	-1.3
85001323	32.3	32.2	0.3
85001321	30.7	30.9	-0.8
85001318	35.4	35.9	-1.4
85001316	30.3	29.9	1.3
85001315	22.3	22.2	0.5
85001313	34.1	34.3	-0.3
85001310	40.0	40.9	-2.2
85001300	36.5	37.0	-1.4
85001300	40.2	41.6	-3.4
85001304	35.4	37.1	-4.6
90000295	40.9	42.6	-4.0
90000296	40.8	39.5	3.3
85001300	35.4	36.1	-4.5
85001317	34.8	35.3	-1.4
85001300	35.3	37.8	-6.8

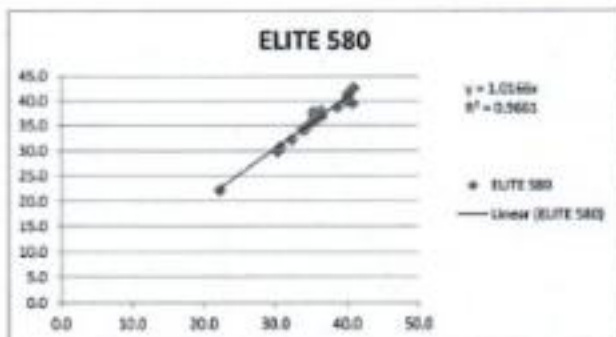

Company Representative

Sig: *[Signature]*

Date: 10/16/20



Customer Authorization

Sig: *[Signature]*

Date: 10/16/20

INSTITUTE NAME


DR B LAL CLINICAL LABORATORY

Instrument Serial Number: _____ K11051912060

Inter Instrument Comparison-HGB

Date performed:

SID NO.	XS	ELITE 580	% BIAS
85001330	13.0	13.1	-0.8
85001329	13.5	13.7	-1.5
85001325	11.6	11.8	-1.7
85001323	10.0	10.9	-8.3
85001321	12.2	12.3	-0.8
85001318	12.2	12.3	-0.8
85001316	9.2	9.2	0.0
85001315	6.0	6.1	-1.8
85001313	11.1	11.1	0.0
85001310	13.6	13.6	0.0
85001309	11.8	11.8	0.0
85001308	14.1	14.1	0.0
85001304	12.5	12.6	-0.8
85000205	14.2	14.2	0.0
85000206	13.6	13.7	-0.7
85001303	12.5	12.6	-0.8
85001317	11.6	11.7	-0.9
85001300	12.9	12.8	0.8

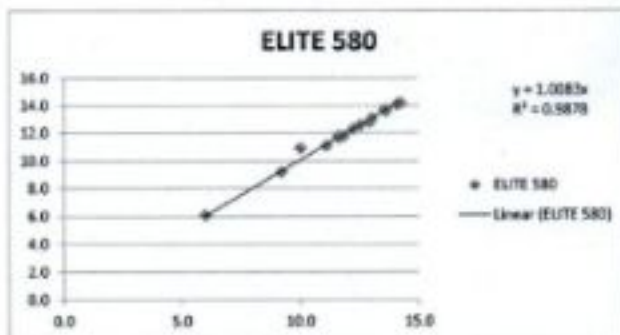

Company Representative

Sig:

Date:



Customer Authorization

Sig:

Date:

Signature
10/6/2020

INSTITUTE NAME


DR B LAL CLINICAL LABORATORY

Instrument Serial Number: _____ K13052912060

Inter Instrument Comparison-RBC

Date performed:

SID NO.	XS	ELITE 580	% BIAS
85001330	4.8	4.8	-0.8
85001329	4.5	4.6	-2.0
85001325	3.9	4.0	-1.5
85001323	4.3	4.4	-2.1
85001321	4.3	4.4	-2.7
85001318	4.5	4.6	-1.5
85001316	4.1	4.2	-2.8
85001315	4.2	4.2	1.0
85001313	3.9	3.8	2.9
85001210	4.8	4.9	-0.8
85001309	4.9	4.8	2.9
85001306	4.8	4.6	3.2
85001304	4.2	4.1	3.4
96000205	4.6	4.4	4.3
96000206	4.5	4.4	3.2
85001303	3.9	3.7	4.9
85001317	4.7	4.6	3.1
85001300	3.7	3.7	-0.8

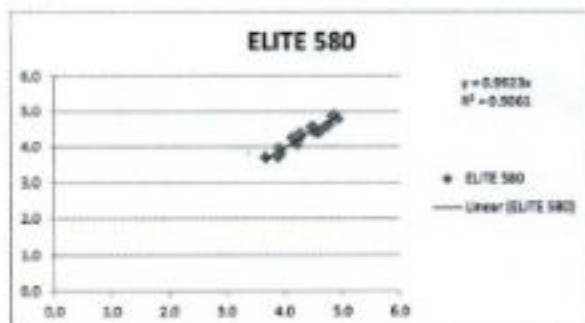

Company Representative

Sng:

Date:

NSCCL
SIGNED CALSLEY

Arjun Lj
10-6-2020

Customer Authorization

Sng:

Date:

Arjun
10/6/2020

INSTITUTE NAME


DR B LAL CLINICAL LABORATORY

Instrument Serial Number: K11051912060

Inter Instrument Comparison-WBC

Date performed:

SID NO.	X5	ELITE 580	% BIAS
85001330	11.8	13.6	-12.8
85001329	8.3	8.0	-7.6
85001325	6.3	7.2	-12.9
85001323	8.2	8.9	-7.5
85001321	12.0	13.4	-10.2
85001318	6.8	7.5	-8.9
85001316	5.3	5.9	-11.0
85001315	5.6	6.3	-10.4
85001313	6.9	7.6	-8.9
85001310	5.4	6.6	-17.5
85001309	9.1	10.7	-14.8
85001308	5.1	5.8	-9.1
85001304	5.6	6.2	-8.8
86000205	4.9	5.7	-13.2
86000205	10.3	11.4	-9.7
85001303	7.3	8.2	-11.7
85001317	9.5	10.3	-7.2
85001300	7.5	8.5	-11.2

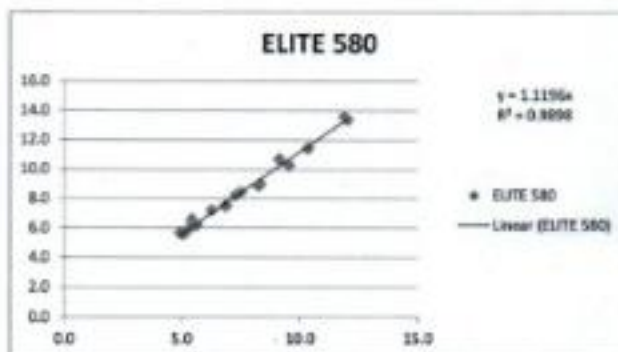

Stm
 10/6/200

Lab Serial No. : RS2006000413	SIN No., Date : RS001330 10-Jun-20 01:16 PM
Patient Name : Mr. ISHAK MOHAMMAD	Sample collection date : 10-Jun-2020 01:16 PM
Referred by : Dr. G.L. Raithi	Report Date : 10-Jun-2020 01:38 PM
Age/Gender : 30 YRS/ M	Report printed on : 10-Jun-2020 02:43 PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	13.1	g/dL	13.0-17.0
Haematocrit (HCT)	38.7	%	40-50
Red Blood Cell Count (RBC)	4.83	million/mm ³	4.5-5.5
Mean Corpuscular Volume (MCV)	80.1	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	27.1	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	33.9	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	14.7	%	11.8-14.5
Total Leucocyte Count (TLC)	11.85	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	73.8	%	42-72
Lymphocytes	14.7	%	25-45
Eosinophils	0.6	%	1-6
Monocytes	10.8	%	2-10
Basophils	0.1	%	<2

Absolute Leucocyte Count

Neutrophils	8.75	1000/mm ³	2.0-7.0
Lymphocytes	1.74	1000/mm ³	1.0-3.0
Eosinophils	0.07	1000/mm ³	0.05-0.50
Monocytes	1.28	1000/mm ³	0.2-1.0
Basophils	0.01	1000/mm ³	0.02-0.2
Platelet count	3.29	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	12.3	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remarks: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200600412	SIN No., Date : 85001329 10-Jun-20 01:11 PM
Patient Name : Mrs. ANITA DEVI	Sample collection date : 10-Jun-2020 01:11 PM
20001509	Report Date : 10-Jun-2020 01:32PM
Referred by : Dr. Jitendra Kacholia	Report printed on : 10-Jun-2020 02:42PM
Age/Gender : 38 YRS / F	
Source IV :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	13.7	g/dL	12.0-15.0
Haematocrit (HCT)	39.3	%	37-46
Red Blood Cell Count (RBC)	4.46	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	88.1	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	30.7	pg	27-32
Mean Corpuscular Haemoglobin Conc. (MCHC)	34.9	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	14.2	%	12.2-16.1
Total Leucocyte Count (TLC)	8.33	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	56.6	%	42-72
Lymphocytes	32.9	%	25-45
Eosinophils	2.8	%	1-6
Monocytes	7.2	%	2-10
Basophils	0.5	%	<2

Absolute Leucocyte Count

Neutrophils	4.72	1000/mm ³	2.0-7.0
Lymphocytes	2.74	1000/mm ³	1.0-3.0
Eosinophils	0.23	1000/mm ³	0.05-0.50
Monocytes	0.60	1000/mm ³	0.2-1.0
Basophils	0.04	1000/mm ³	0.02-0.2
Platelet count	3.21	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	9.4	fL	7.8-11.0

Method : Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytocentrifuge, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 852006000408	SIV No., Date : 85001325 10-Jun-20 12:39 PM
Patient Name : Mrs. NAJMA 20001504	Sample collection date : 10-Jun-2020 12:39 PM
Referred by : Dr. Jitendra Kacholia	Report Date : 10-Jun-2020 01:04PM
Age/Gender : 30 YRS / F	Report printed on : 10-Jun-2020 02:41PM
Source ID :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)

Haemoglobin	11.8	g/dL	12.0-15.0
Haematocrit (HCT)	33.8	%	37-46
Red Blood Cell Count (RBC)	3.91	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	86.4	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	30.2	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	34.9	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	12.7	%	12.2-16.1
Total Leucocyte Count (TLC)	6.27	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	51.9	%	42-72
Lymphocytes	35.1	%	25-45
Eosinophils	4.9	%	1-6
Monocytes	7.8	%	2-10
Basophils	0.3	%	<2

Absolute Leucocyte Count

Neutrophils	3.25	1000/mm ³	2.0-7.0
Lymphocytes	2.20	1000/mm ³	1.0-3.0
Eosinophils	0.31	1000/mm ³	0.05-0.50
Monocytes	0.49	1000/mm ³	0.2-1.0
Basophils	0.02	1000/mm ³	0.02-0.2
Platelet count	3.19	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	10.3	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 852006000406	SIN No., Date : 85001323 10-Jun-20 12:31 PM
Patient Name : Ms. ALVEERA KHANAM	Sample collection date : 10-Jun-2020 12:31 PM
20001506	
Referred by : Dr. Jitendra Kaushik	Report Date : 10-Jun-2020 12:52PM
Age/Gender : 10 YRS / F	Report printed on : 10-Jun-2020 02:41PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	10.9	g/dL	11.5-15.5
Haematocrit (HCT)	32.3	%	35-45
Red Blood Cell Count (RBC)	4.28	million/mm ³	4.0-5.2
Mean Corpuscular Volume (MCV)	75.5	fL	77-96
Mean Corpuscular Haemoglobin (MCH)	25.5	pg	25-33
Mean Corpuscular Haemoglobin Conc.(MCHC)	33.7	g/dL	31-37
Red Cell Distribution Width (RDWcv)	14.1	%	11.4-13.5
Total Leucocyte Count (TLC)	8.22	1000/mm ³	5.0-13.0

Differential Leucocyte Count

Segmented Neutrophils	36.7	%	38-58
Lymphocytes	50.7	%	25-54
Eosinophils	5.2	%	1-6
Monocytes	6.9	%	2-10
Basophils	0.5	%	<2

Absolute Leucocyte Count

Neutrophils	3.01	1000/mm ³	1.5-8.5
Lymphocytes	4.17	1000/mm ³	1.5-6.5
Eosinophils	0.43	1000/mm ³	0.0-0.50
Monocytes	0.57	1000/mm ³	0.2-1.0
Basophils	0.04	1000/mm ³	0.02-0.2
Platelet count	3.76	Lakhs/cumm	1.8-4.0
Mean Platelet Volume (MPV)	9.3	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 852006000404	SIR No., Date : 85001321 10-Jun-20 12:20 PM
Patient Name : Mrs. LICHAMI 18082792	Sample collection date : 10-Jun-2020 12:20 PM
Referred by : Dr. Anita Rathi	Report Date : 10-Jun-2020 12:52PM
Age/Gender : 25 YRS / F	Report printed on : 10-Jun-2020 02:41PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	10.1	g/dL	12.0-15.0
Haematocrit (HCT)	30.7	%	37-48
Red Blood Cell Count (RBC)	4.27	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	71.9	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	23.7	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	32.9	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	23.0	%	12.2-16.1
Total Leucocyte Count (TLC)	12.02	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	75.0	%	42-72
Lymphocytes	19.7	%	25-45
Eosinophils	0.7	%	1-6
Monocytes	4.4	%	2-10
Basophils	0.2	%	<2

Absolute Leucocyte Count

Neutrophils	9.02	1000/mm ³	2.0-7.0
Lymphocytes	2.37	1000/mm ³	1.0-3.0
Eosinophils	0.08	1000/mm ³	0.05-0.50
Monocytes	0.53	1000/mm ³	0.2-1.0
Basophils	0.02	1000/mm ³	0.02-0.2
Platelet count	2.83	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	9.9	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytocentrifugation, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. **852806800401** S/N No., Date : **85001318 10-Jun-20 11:32 AM**
 Patient Name **Mrs. RUKSANA 2001497** Sample collection date : **10-Jun-2020 11:32 AM**
 Referred by **Dr. G.L.Rathi** Report Date : **10-Jun-2020 12:00PM**
 Age/Gender **30 YRS / F** Report printed on : **10-Jun-2020 02:40PM**
 Source ID :

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	12.3	g/dL	12.0-15.0
Haematocrit (HCT)	35.4	%	37-46
Red Blood Cell Count (RBC)	4.48	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	78.8	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	27.4	pg	27-32
Mean Corpuscular Haemoglobin Conc. (MCHC)	34.7	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	14.9	%	12.2-16.1
Total Leucocyte Count (TLC)	6.94	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	57.7	%	42-72
Lymphocytes	31.3	%	25-45
Eosinophils	4.5	%	1-6
Monocytes	5.8	%	2-10
Basophils	0.7	%	<2

Absolute Leucocyte Count

Neutrophils	3.94	1000/mm ³	2.0-7.0
Lymphocytes	2.14	1000/mm ³	1.0-3.0
Eosinophils	0.31	1000/mm ³	0.05-0.50
Monocytes	0.40	1000/mm ³	0.2-1.0
Basophils	0.05	1000/mm ³	0.02-0.2
Platelet count	4.19	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	10.2	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytocentrifuge, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200600399	SNV No., Date : 85001316 10-Jun-20 11:22 AM
Patient Name : Mrs. RUKSANA 20000603	Sample collection date : 10-Jun-2020 11:22 AM
Referred by : Dr. Anita Rathil	Report Date : 10-Jun-2020 12:00PM
Age/Gender : 35 YRS / F	Report printed on : 10-Jun-2020 02:40PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)

Haemoglobin	9.2	g/dL	12.0-15.0
Haematocrit (HCT)	30.3	%	37-46
Red Blood Cell Count (RBC)	4.13	million/mm3	3.8-4.8
Mean Corpuscular Volume (MCV)	73.4	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	22.3	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	30.4	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	17.7	%	12.2-16.1
Total Leucocyte Count (TLC)	5.26	1000/mm3	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	56.0	%	42-72
Lymphocytes	32.9	%	25-45
Eosinophils	1.9	%	1-6
Monocytes	8.6	%	2-10
Basophils	0.6	%	<2

Absolute Leucocyte Count

Neutrophils	2.95	1000/mm3	2.0-7.0
Lymphocytes	1.73	1000/mm3	1.0-3.0
Eosinophils	0.10	1000/mm3	0.05-0.50
Monocytes	0.45	1000/mm3	0.2-1.0
Basophils	0.03	1000/mm3	0.02-0.2
Platelet count	1.54	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	11.9	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200600398	SIN No., Date : 85001315 10-Jun-20 11:16 AM
Patient Name : Mrs. NAJMA BANO	Sample collection date : 10-Jun-2020 11:16 AM
Referred by : Dr. Divya Kacholia	Report Date : 10-Jun-2020 12:00PM
Age/Gender : 40 YRS / F	Report printed on : 10-Jun-2020 02:40PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	6.1	g/dL	12.0-15.0
Haematocrit (HCT)	22.3	%	37-46
Red Blood Cell Count (RBC)	4.24	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	52.6	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	14.4	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	27.4	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	22.1	%	12.2-18.1
Total Leucocyte Count (TLC)	5.61	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	70.4	%	42-72
Lymphocytes	22.3	%	25-45
Eosinophils	0.5	%	1-6
Monocytes	6.1	%	2-10
Basophils	0.7	%	<2

Absolute Leucocyte Count

Neutrophils	3.95	1000/mm ³	2.0-7.0
Lymphocytes	1.25	1000/mm ³	1.0-3.0
Eosinophils	0.03	1000/mm ³	0.05-0.50
Monocytes	0.34	1000/mm ³	0.2-1.0
Basophils	0.04	1000/mm ³	0.02-0.2
Platelet count	5.34	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	9.1	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 852006000396	SIN No., Date : 85001313 10-Jun-20 11:13 AM
Patient Name : Mrs. KISMAT BANO 19021808	Sample collection date : 10-Jun-2020 11:13 AM
Referred by : Dr. Anilash Rathi	Report Date : 10-Jun-2020 12:00PM
Age/Gender : 38 YRS / F	Report printed on : 10-Jun-2020 02:39PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	11.1	g/dL	12.0-15.0
Haematocrit (HCT)	34.1	%	37-48
Red Blood Cell Count (RBC)	3.83	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	89.0	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	29.0	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	32.6	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	14.3	%	12.2-16.1
Total Leucocyte Count (TLC)	6.88	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	53.4	%	42-72
Lymphocytes	31.5	%	25-45
Eosinophils	1.0	%	1-6
Monocytes	13.5	%	2-10
Basophils	0.6	%	<2

Absolute Leucocyte Count

Neutrophils	3.67	1000/mm ³	2.0-7.0
Lymphocytes	2.17	1000/mm ³	1.0-3.0
Eosinophils	0.07	1000/mm ³	0.05-0.50
Monocytes	0.93	1000/mm ³	0.2-1.0
Basophils	0.04	1000/mm ³	0.02-0.2
Platelet count	4.51	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	10.0	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additional being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 852006000393	SIN No., Date : 85001310 10-Jun-20 10:57 AM
Patient Name : Mr. TEJPAL SAINI 20001485	Sample collection date : 10-Jun-2020 10:57 AM
Referred by : Dr. G.L.Rathi	Report Date : 10-Jun-2020 12:08PM
Age/Gender : 35 YRS / M	Report printed on : 10-Jun-2020 02:39PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)			
Haemoglobin	13.6	g/dL	13.0-17.0
Haematocrit (HCT)	40.0	%	40-50
Red Blood Cell Count (RBC)	4.75	million/mm ³	4.5-5.5
Mean Corpuscular Volume (MCV)	84.2	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	28.6	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	34.0	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	15.2	%	11.8-14.5
Total Leucocyte Count (TLC)	5.43	1000/mm ³	4.0-10.0
Differential Leucocyte Count			
Segmented Neutrophils	58.1	%	42-72
Lymphocytes	32.6	%	25-45
Eosinophils	1.5	%	1-6
Monocytes	7.6	%	2-10
Basophils	0.2	%	<2
Absolute Leucocyte Count			
Neutrophils	3.16	1000/mm ³	2.0-7.0
Lymphocytes	1.77	1000/mm ³	1.0-3.0
Eosinophils	0.08	1000/mm ³	0.05-0.50
Monocytes	0.41	1000/mm ³	0.2-1.0
Basophils	0.01	1000/mm ³	0.02-0.2
Platelet count	0.86	Lakhs/cumm	1.5-4.0

few large platelets seen and counts are adequate on smear.(approximately 1.5L/cumm)

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 852006000392	SIV No., Date : 85001309 10-Jun-20 10:48 AM
Patient Name : Mrs. SANTOSH 2000324	Sample collection date : 10-Jun-2020 10:48 AM
Referred by : Dr. Anush Rath	Report Date : 10-Jun-2020 11:57AM
Age/Gender : 63 YRS / F	Report printed on : 10-Jun-2020 02:39PM
Source Ref :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)

Haemoglobin	11.8	g/dL	12.0-15.0
Haematocrit (HCT)	36.5	%	37-48
Red Blood Cell Count (RBC)	4.79	million/mm ³	3.8-4.8
Mean Corpuscular Volume (MCV)	76.2	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	24.6	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	32.3	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	18.9	%	12.2-16.1
Total Leucocyte Count (TLC)	9.13	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	60.5	%	42-72
Lymphocytes	28.1	%	25-45
Eosinophils	3.3	%	1-6
Monocytes	7.9	%	2-10
Basophils	0.2	%	<2

Absolute Leucocyte Count

Neutrophils	5.52	1000/mm ³	2.0-7.0
Lymphocytes	2.57	1000/mm ³	1.0-3.0
Eosinophils	0.30	1000/mm ³	0.05-0.50
Monocytes	0.72	1000/mm ³	0.2-1.0
Basophils	0.02	1000/mm ³	0.02-0.2
Platelet count	3.83	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	11.8	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are automatically being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200600389	SUN No., Date : 85001306 10-Jun-20 10:27 AM
Patient Name : Mr. VIJENDRA SINGH RATHORE 20001488	Sample collection date : 10-Jun-2020 10:27 AM
Referred by : Dr. Jitendra Kacholia	Report Date : 10-Jun-2020 11:37AM
Age/Gender : 28 YRS / M	Report printed on : 10-Jun-2020 02:38PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)

Haemoglobin	14.1	g/dL	13.0-17.0
Haematocrit (HCT)	40.2	%	40-50
Red Blood Cell Count (RBC)	4.62	million/mm3	4.5-5.5
Mean Corpuscular Volume (MCV)	87.0	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	30.5	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	35.1	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	13.9	%	11.8-14.5
Total Leucocyte Count (TLC)	5.10	1000/mm3	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	48.8	%	42-72
Lymphocytes	41.2	%	25-45
Eosinophils	1.8	%	1-6
Monocytes	7.8	%	2-10
Basophils	0.4	%	<2

Absolute Leucocyte Count

Neutrophils	2.49	1000/mm3	2.0-7.0
Lymphocytes	2.10	1000/mm3	1.0-3.0
Eosinophils	0.09	1000/mm3	0.05-0.50
Monocytes	0.40	1000/mm3	0.2-1.0
Basophils	0.02	1000/mm3	0.02-0.2
Platelet count	3.18	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	9.7	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200600387	Slr No., Date : 8501304 10-Jun-20 10:14 AM
Patient Name : Mrs. AMREEN BANO	Sample collection date : 10-Jun-2020 10:14 AM
Referred by : Dr. Jitendra Kachola	Report Date : 10-Jun-2020 11:37AM
Age/Gender : 22 YRS / F	Report printed on : 10-Jun-2020 02:18PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)

Haemoglobin	12.6	g/dL	12.0-15.0
Haematocrit (HCT)	35.4	%	37-46
Red Blood Cell Count (RBC)	4.07	million/mm ³	3.8-4.5
Mean Corpuscular Volume (MCV)	87.0	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	31.0	pg	27-32
Mean Corpuscular Haemoglobin Conc. (MCHC)	35.6	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	13.7	%	12.2-16.1
Total Leucocyte Count (TLC)	5.62	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	56.2	%	42-72
Lymphocytes	33.8	%	25-45
Eosinophils	0.5	%	1-6
Monocytes	9.3	%	2-10
Basophils	0.2	%	<2

Absolute Leucocyte Count

Neutrophils	3.16	1000/mm ³	2.0-7.0
Lymphocytes	1.90	1000/mm ³	1.0-3.0
Eosinophils	0.03	1000/mm ³	0.05-0.50
Monocytes	0.52	1000/mm ³	0.2-1.0
Basophils	0.01	1000/mm ³	0.02-0.2
Platelet count	1.65	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	13.0	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per cent volume of blood.

*** End of report ***



Lab Serial No. : 96200600072	Slr No., Date : 9600205 10-Jun-20 08:05 AM
Patient Name : Mr. SHANKAR LAL	Sample collection date : 10-Jun-2020 08:05 AM
Referred by : Dr. SELF	Report Date : 10-Jun-2020 11:46AM
Age/Gender : 47 YRS / M	Report printed on : 10-Jun-2020 02:50PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	14.2	g/dL	13.0-17.0
Haematocrit (HCT)	40.9	%	40-50
Red Blood Cell Count (RBC)	4.41	million/mm ³	4.5-5.5
Mean Corpuscular Volume (MCV)	92.7	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	32.2	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	34.7	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	12.8	%	11.8-14.5
Total Leucocyte Count (TLC)	4.92	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	50.7	%	42-72
Lymphocytes	34.3	%	25-45
Eosinophils	6.1	%	1-6
Monocytes	8.1	%	2-10
Basophils	0.8	%	<2

Absolute Leucocyte Count

Neutrophils	2.49	1000/mm ³	2.0-7.0
Lymphocytes	1.69	1000/mm ³	1.0-3.0
Eosinophils	0.30	1000/mm ³	0.05-0.50
Monocytes	0.40	1000/mm ³	0.2-1.0
Basophils	0.04	1000/mm ³	0.02-0.2
Platelet count	1.83	Lakhs/cumm	1.5-4.0

Method : Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 962006000073	SN No., Date : 96000206 10-Jun-20 08:19 AM
Patient Name : Mr. BHAGIRATH MAL	Sample collection date : 10-Jun-2020 08:19 AM
Referred by : Dr. R.M. MATHUR	Report Date : 10-Jun-2020 11:38AM
Age/Gender : 65 YRS / M	Report printed on : 10-Jun-2020 02:51PM
Source BV : 1	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)

Haemoglobin	13.7	g/dL	13.0-17.0
Haematocrit (HCT)	39.5	%	40-50
Red Blood Cell Count (RBC)	4.40	million/mm ³	4.5-5.5
Mean Corpuscular Volume (MCV)	89.8	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	31.1	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	34.7	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	15.0	%	11.8-14.5
Total Leucocyte Count (TLC)	10.33	1000/mm ³	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	70.8	%	42-72
Lymphocytes	19.7	%	26-45
Eosinophils	1.3	%	1-6
Monocytes	9.1	%	2-10
Basophils	0.3	%	<2

Absolute Leucocyte Count

Neutrophils	7.30	1000/mm ³	2.0-7.0
Lymphocytes	1.93	1000/mm ³	1.0-3.0
Eosinophils	0.13	1000/mm ³	0.05-0.50
Monocytes	0.94	1000/mm ³	0.2-1.0
Basophils	0.03	1000/mm ³	0.02-0.2
Platelet count	1.52	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	13.4	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytocentrifugation, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200000356	SIN No., Date : 85001303 10-Jun-20 10:00 AM
Patient Name : Mrs. MEERA DEVI	Sample collection date : 10-Jun-2020 10:00 AM
20001478	
Referred by : Dr. Jitendra Kacholia	Report Date : 10-Jun-2020 11:37AM
Age/Gender : 45 YRS / F	Report printed on : 10-Jun-2020 02:34PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. interval
COMPLETE BLOOD COUNT [CBC/HAEMOGRAM]			
Haemoglobin	12.6	g/dL	12.0-15.0
Haematocrit (HCT)	36.4	%	37-46
Red Blood Cell Count (RBC)	3.71	million/mm ³	3.6-4.8
Mean Corpuscular Volume (MCV)	98.1	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	34.0	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	34.6	g/dL	31.6-34.5
Red Cell Distribution Width (RDWcv)	16.5	%	12.2-16.1
Total Leucocyte Count (TLC)	7.27	1000/mm ³	4.0-10.0
Differential Leucocyte Count			
Segmented Neutrophils	52.2	%	42-72
Lymphocytes	36.0	%	25-45
Eosinophils	3.3	%	1-6
Monocytes	8.4	%	2-10
Basophils	0.1	%	<2
Absolute Leucocyte Count			
Neutrophils	3.79	1000/mm ³	2.0-7.0
Lymphocytes	2.62	1000/mm ³	1.0-3.0
Eosinophils	0.24	1000/mm ³	0.05-0.50
Monocytes	0.61	1000/mm ³	0.2-1.0
Basophils	0.01	1000/mm ³	0.02-0.2
Platelet count	1.22	Lakhs/cumm	1.5-4.0
few large platelets seen and counts are adequate on smear.(approximately 1.8L/cumm)			
Mean Platelet Volume (MPV)	13.2	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytocentrifuge, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85206600400	SIN No., Date : 85001317 10-Jun-20 11:30 AM
Patient Name : Mrs. POOJA DEVI 18080096	Sample collection date : 10-Jun-2020 11:30 AM
Referred by : Dr. Anita Rathbi	Report Date : 10-Jun-2020 12:01PM
Age/Gender : 27 YRS / F	Report printed on : 10-Jun-2020 02:32PM
Source BY :	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
COMPLETE BLOOD COUNT(CBC/HAEMOGRAM)			
Haemoglobin	11.7	g/dL	12.0-15.0
Haematocrit (HCT)	34.8	%	37-46
Red Blood Cell Count (RBC)	4.57	million/mm3	3.8-4.8
Mean Corpuscular Volume (MCV)	76.1	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	25.6	pg	27-32
Mean Corpuscular Haemoglobin Conc.(MCHC)	33.6	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	16.8	%	12.2-16.1
Total Leucocyte Count (TLC)	9.53	1000/mm3	4.0-10.0
Differential Leucocyte Count			
Segmented Neutrophils	65.4	%	42-72
Lymphocytes	26.9	%	25-45
Eosinophils	0.9	%	1-6
Monocytes	6.7	%	2-10
Basophils	0.1	%	<2
Absolute Leucocyte Count			
Neutrophils	6.23	1000/mm3	2.0-7.0
Lymphocytes	2.56	1000/mm3	1.0-3.0
Eosinophils	0.09	1000/mm3	0.05-0.50
Monocytes	0.64	1000/mm3	0.2-1.0
Basophils	0.01	1000/mm3	0.02-0.2
Platelet count	3.14	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	12.7	fL	7.8-11.0

Method: Tests done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



Lab Serial No. : 85200600383	SIN No., Date : 85001300 10-Jun-20 06:30 AM
Patient Name : Mr. KESHAR DEV 200001135	Sample collection date : 10-Jun-2020 06:30 AM
Referred by : Dr. JITENDRA KACHOLIA	Report Date : 10-Jun-2020 07:14AM
Age/Gender : 66 YRS / M	Report printed on : 10-Jun-2020 02:33PM
Source BY : Night Hos. Sibar	

HAEMATOLOGY

Test Name	Observation	Unit	Biological Ref. Interval
-----------	-------------	------	--------------------------

COMPLETE BLOOD COUNT (CBC/HAEMOGRAM)

Haemoglobin	12.8	g/dL	13.0-17.0
Haematocrit (HCT)	35.3	%	40-50
Red Blood Cell Count (RBC)	3.51	million/mm3	4.5-5.5
Mean Corpuscular Volume (MCV)	100.6	fL	83-101
Mean Corpuscular Haemoglobin (MCH)	36.5	pg	27-32
Mean Corpuscular Haemoglobin Conc (MCHC)	36.3	g/dL	31.5-34.5
Red Cell Distribution Width (RDWcv)	17.1	%	11.8-14.5
Total Leucocyte Count (TLC)	7.50	1000/mm3	4.0-10.0

Differential Leucocyte Count

Segmented Neutrophils	69.9	%	42-72
Lymphocytes	22.5	%	25-45
Eosinophils	2.5	%	1-6
Monocytes	5.1	%	2-10
Basophils	0.0	%	<2

Absolute Leucocyte Count

Neutrophils	5.24	1000/mm3	2.0-7.0
Lymphocytes	1.69	1000/mm3	1.0-3.0
Eosinophils	0.19	1000/mm3	0.05-0.50
Monocytes	0.38	1000/mm3	0.2-1.0
Basophils	0.00	1000/mm3	0.02-0.2
Platelet count	1.15	Lakhs/cumm	1.5-4.0
Mean Platelet Volume (MPV)	13.3	fL	7.8-11.0

Method: Test done by EDTA sample on automated cell counter, based on Electrical Impedance, Cytochemistry, Spectrophotometry & Microscopy.

Remark: As per the recommendation of International Council for Standardization in Hematology, the differential leucocyte counts are additionally being reported as absolute numbers of each cell in per unit volume of blood.

*** End of report ***



DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001330
Run Time: 2020/06/10 08:19
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	13.59 ↑	4.00-10.00	10 ³ /uL	16 RBC	4.87	3.50-5.50	10 ⁶ /uL
2 Neu%	74.4 ↑	50.0-70.0	%	17 HGB	13.0	11.0-16.0	g/dL
3 Lym%	15.2 ↓	20.0-40.0	%	18 HCT	38.7	37.0-54.0	%
4 Mon%	9.6	3.0-12.0	%	19 MCV	79.3 ↓	80.0-100.0	fL
5 Eos%	0.5	0.5-5.0	%	20 MCH	26.6 ↓	27.0-34.0	pg
6 Bas%	0.3	0.0-1.0	%	21 MCHC	33.6	32.0-36.0	g/dL
7 Neu#	10.11 ↑	2.00-7.00	10 ³ /uL	22 RDW-CV	14.2	11.0-16.0	%
8 Lym#	2.07	0.80-4.00	10 ³ /uL	23 RDW-SD	40.3	35.0-56.0	fL
9 Mon#	1.30 ↑	0.12-1.20	10 ³ /uL	24 PLT	331 ↑	100-300	10 ³ /uL
10 Eos#	0.07	0.02-0.50	10 ³ /uL	25 MPV	12.2 ↑	6.5-12.0	fL
11 Bact#	0.04	0.00-0.10	10 ³ /uL	26 PCT	0.404 ↑	0.108-0.282	%
12 *ALY#	0.05	0.00-0.20	10 ³ /uL	27 P-LCR	41.4	11.0-45.0	%
13 *ALY%	0.4	0.0-2.0	%	28 P-LCC	137 ↑	30-90	10 ⁹ /L
14 *LIC#	0.01	0.00-0.20	10 ³ /uL				
15 *LIC%	0.1	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:19

Delivery Time: 2020/06/10 08:19

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:

Sample Type:

Sample ID: invalid2

Last Name:

Department:

Run Time: 2020/06/10 08:20

Gender:

Patient ID: 85001329

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	9.02	4.00-10.00	10 ³ /uL	16 RBC	4.55	3.50-5.50	10 ⁶ /uL
2 Neu%	60.0	50.0-70.0	%	17 HGB	13.5	11.0-16.0	g/dL
3 Lym%	32.2	20.0-40.0	%	18 HCT	39.9	37.0-54.0	%
4 Mon%	5.1	3.0-12.0	%	19 MCV	87.7	80.0-100.0	fL
5 Eos%	2.5	0.5-5.0	%	20 MCH	29.7	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	33.8	32.0-36.0	g/dL
7 Neut#	5.41	2.00-7.00	10 ³ /uL	22 RDW-CV	14.3	11.0-16.0	%
8 Lym#	2.90	0.80-4.00	10 ³ /uL	23 RDW-SD	44.5	35.0-56.0	fL
9 Mon#	0.46	0.12-1.20	10 ³ /uL	24 PLT	324	100-300	10 ³ /uL
10 Eos#	0.23	0.02-0.50	10 ³ /uL	25 MPV	8.8	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.264	0.108-0.282	%
12 *ALY#	0.08	0.00-0.20	10 ³ /uL	27 P-LCR	17.8	11.0-45.0	%
13 *ALY%	0.8	0.0-2.0	%	28 P-LCC	58	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:20

Delivery Time: 2020/06/10 08:20

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001325
Run Time: 2020/06/10 08:18
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	7.20	4.00-10.00	10 ³ /uL	16 RBC	3.97	3.50-5.50	10 ⁶ /uL
2 Neu%	53.3	50.0-70.0	%	17 HGB	11.6	11.0-16.0	g/dL
3 Lym%	35.1	20.0-40.0	%	18 HCT	34.2	37.0-54.0	%
4 Mon%	7.0	3.0-12.0	%	19 MCV	86.0	80.0-100.0	fL
5 Eos%	4.3	0.5-5.0	%	20 MCH	29.3	27.0-34.0	pg
6 Bas%	0.3	0.0-1.0	%	21 MCHC	34.0	32.0-36.0	g/dL
7 Neu#	3.84	2.00-7.00	10 ³ /uL	22 RDW-CV	13.1	11.0-16.0	%
8 Lym#	2.53	0.80-4.00	10 ³ /uL	23 RDW-SD	40.2	35.0-56.0	fL
9 Mon#	0.50	0.12-1.20	10 ³ /uL	24 PLT	336	100-300	10 ³ /uL
10 Eos#	0.31	0.02-0.50	10 ³ /uL	25 MPV	10.3	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.347	0.108-0.282	%
12 *ALY#	0.07	0.00-0.20	10 ³ /uL	27 P-LCR	28.4	11.0-45.0	%
13 *ALY%	0.9	0.0-2.0	%	28 P-LCC	96	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam, Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:18

Delivery Time: 2020/06/10 08:18

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001323
Run Time: 2020/06/10 08:18
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	8.89	4.00-10.00	10 ³ /uL	16 RBC	4.37	3.50-5.50	10 ⁶ /uL
2 Neu%	38.5 ↓	50.0-70.0	%	17 HGB	10.8 ↓	11.0-16.0	g/dL
3 Lym%	51.0 ↑	20.0-40.0	%	18 HCT	32.2 ↓	37.0-54.0	%
4 Mon%	5.9	3.0-12.0	%	19 MCV	73.6 ↓	80.0-100.0	fL
5 Eos%	4.3	0.5-5.0	%	20 MCH	24.8 ↓	27.0-34.0	pg
6 Bas%	0.3	0.0-1.0	%	21 MCHC	33.7	32.0-36.0	g/dL
7 Neu#	3.42	2.00-7.00	10 ³ /uL	22 RDW-CV	14.5	11.0-16.0	%
8 Lym#	4.54 ↑	0.80-4.00	10 ³ /uL	23 RDW-SD	38.1	35.0-56.0	fL
9 Mon#	0.52	0.12-1.20	10 ³ /uL	24 PLT	385 ↑	100-300	10 ³ /uL
10 Eos#	0.38	0.02-0.50	10 ³ /uL	25 MPV	9.2	6.5-12.0	fL
11 Bas#	0.03	0.00-0.10	10 ³ /uL	26 PCT	0.354 ↑	0.108-0.282	%
12 *ALY#	0.11	0.00-0.20	10 ³ /uL	27 P-LCR	19.8	11.0-45.0	%
13 *ALY%	1.2	0.0-2.0	%	28 P-LCC	76	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:18

Delivery Time: 2020/06/10 08:18

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001321
Run Time: 2020/06/10 08:17
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	13.39 ↑	4.00-10.00	10 ³ /uL	16 RBC	4.39	3.50-5.50	10 ⁶ /uL
2 Neu%	78.0 ↓	50.0-70.0	%	17 HGB	10.0 ↓	11.0-16.0	g/dL
3 Lym%	19.5 ↓	20.0-40.0	%	18 HCT	30.9 ↓	37.0-54.0	%
4 Mon%	3.8	3.0-12.0	%	19 MCV	70.4 ↓	80.0-100.0	fL
5 Eos%	0.5	0.5-5.0	%	20 MCH	22.7 ↓	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	32.3	32.0-36.0	g/dL
7 Neu#	10.17 ↑	2.00-7.00	10 ³ /uL	22 RDW-CV	23.4 ↑	11.0-16.0	%
8 Lym#	2.61	0.80-4.00	10 ³ /uL	23 RDW-SD	58.9 ↑	35.0-56.0	fL
9 Mon#	0.51	0.12-1.20	10 ³ /uL	24 PLT	304 ↓	100-300	10 ³ /uL
10 Eos#	0.07	0.02-0.50	10 ³ /uL	25 MPV	9.6	6.5-12.0	fL
11 Bas#	0.03	0.00-0.10	10 ³ /uL	26 PCT	0.293 ↑	0.108-0.282	%
12 *ALY#	0.08	0.00-0.20	10 ³ /uL	27 P-LCR	24.5	11.0-45.0	%
13 *ALY%	0.6	0.0-2.0	%	28 P-LCC	74	30-90	10 ⁹ /L
14 *LIC#	0.01	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

**** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:17

Delivery Time: 2020/06/10 08:17

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001318
Run Time: 2020/06/10 08:16
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	7.51	4.00-10.00	10 ³ /uL	16 RBC	4.56	3.50-5.50	10 ⁶ /uL
2 Neu%	58.5	50.0-70.0	%	17 HGB	12.2	11.0-16.0	g/dL
3 Lym%	32.4	20.0-40.0	%	18 HCT	35.9 ↓	37.0-54.0	%
4 Mon%	4.7	3.0-12.0	%	19 MCV	78.8 ↓	80.0-100.0	fL
5 Eos%	4.2	0.5-5.0	%	20 MCH	26.7 ↓	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	33.9	32.0-36.0	g/dL
7 Neut#	4.39	2.00-7.00	10 ³ /uL	22 RDW-CV	14.8	11.0-16.0	%
8 Lym#	2.43	0.80-4.00	10 ³ /uL	23 RDW-SD	41.6	35.0-56.0	fL
9 Mon#	0.35	0.12-1.20	10 ³ /uL	24 PLT	411 ↑	100-300	10 ³ /uL
10 Eos#	0.32	0.02-0.50	10 ³ /uL	25 MPV	10.2	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.422 ↑	0.108-0.282	%
12 *ALY#	0.07	0.00-0.20	10 ³ /uL	27 P-LCR	27.2	11.0-45.0	%
13 *ALY%	0.9	0.0-2.0	%	28 P-LCC	112 ↑	30-90	10 ⁹ /L
14 *LIC#	0.01	0.00-0.20	10 ³ /uL				
15 *LIC%	0.1	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:16

Delivery Time: 2020/06/10 08:16

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID: 85001316

Sample ID: invalid1
Run Time: 2020/06/10 08:14
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	5.91	4.00-10.00	10 ³ /uL	16 RBC	4.25	3.50-5.50	10 ⁶ /uL
2 Neu%	55.4	50.0-70.0	%	17 HGB	9.2 ↓	11.0-16.0	g/dL
3 Lym%	35.5	20.0-40.0	%	18 HCT	29.9 ↓	37.0-54.0	%
4 Mon%	7.7	3.0-12.0	%	19 MCV	70.5 ↓	80.0-100.0	fL
5 Eos%	1.2	0.5-5.0	%	20 MCH	21.6 ↓	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	30.7 ↓	32.0-36.0	g/dL
7 Neut#	3.27	2.00-7.00	10 ³ /uL	22 RDW-CV	17.9 ↑	11.0-16.0	%
8 Lym#	2.10	0.80-4.00	10 ³ /uL	23 RDW-SD	45.2	35.0-56.0	fL
9 Mon#	0.46	0.12-1.20	10 ³ /uL	24 PLT	163	100-300	10 ³ /uL
10 Eos#	0.07	0.02-0.50	10 ³ /uL	25 MPV	12.1 ↑	6.5-12.0	fL
11 Bas#	0.01	0.00-0.10	10 ³ /uL	26 PCT	0.198	0.108-0.282	%
12*ALY#	0.03	0.00-0.20	10 ³ /uL	27 P-LCR	41.2	11.0-45.0	%
13*ALY%	0.5	0.0-2.0	%	28 P-LCC	67	30-90	10 ⁹ /L
14*LIC#	0.00	0.00-0.20	10 ³ /uL				
15*LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam, Time:

Submitter: Operator: admin Approver: service
 Sampling Time: 2020/06/10 08:14 Delivery Time: 2020/06/10 08:14 Validated Time: 2020/06/10 08:38
 Report Time: 2020/06/10 08:37 Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001315
Run Time: 2020/06/10 08:13
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	6.26	4.00-10.00	10 ³ /uL	16 RBC	4.44	3.50-5.50	10 ⁶ /uL
2 Neu%	71.6 ↑	50.0-70.0	%	17 HGB	6.0 ↓	11.0-16.0	g/dL
3 Lym%	23.4	20.0-40.0	%	18 HCT	22.2 ↓	37.0-54.0	%
4 Mon%	4.7	3.0-12.0	%	19 MCV	49.9 ↓	80.0-100.0	fL
5 Eos%	0.1 ↓	0.5-5.0	%	20 MCH	13.6 ↓	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	27.3 ↓	32.0-36.0	g/dL
7 Neu#	4.49	2.00-7.00	10 ³ /uL	22 RDW-CV	21.1 ↑	11.0-16.0	%
8 Lym#	1.46	0.80-4.00	10 ³ /uL	23 RDW-SD	37.8	35.0-56.0	fL
9 Mon#	0.29	0.12-1.20	10 ³ /uL	24 PLT	530 ↑	100-300	10 ³ /uL
10 Eos#	0.01 ↓	0.02-0.50	10 ³ /uL	25 MPV	8.8	6.5-12.0	fL
11 Bas#	0.01	0.00-0.10	10 ³ /uL	26 PCT	0.467 ↑	0.108-0.282	%
12 *ALY#	0.02	0.00-0.20	10 ³ /uL	27 P-LCR	19.5	11.0-45.0	%
13 *ALY%	0.3	0.0-2.0	%	28 P-LCC	103 ↑	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means *Research use only, not for diagnostic use*.

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:13

Delivery Time: 2020/06/10 08:13

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:

Sample Type:

Sample ID: 85001313

Last Name:

Department:

Run Time: 2020/06/10 08:13

Gender:

Patient ID:

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	7.55	4.00-10.00	10 ³ /uL	16 RBC	3.94	3.50-5.50	10 ⁶ /uL
2 Neu%	53.7	50.0-70.0	%	17 HGB	11.1	11.0-16.0	g/dL
3 Lym%	33.8	20.0-40.0	%	18 HCT	34.2	37.0-54.0	%
4 Mon%	11.5	3.0-12.0	%	19 MCV	86.6	80.0-100.0	fL
5 Eos%	0.5	0.5-5.0	%	20 MCH	28.0	27.0-34.0	pg
6 Bas%	0.5	0.0-1.0	%	21 MCHC	32.4	32.0-36.0	g/dL
7 Neut#	4.05	2.00-7.00	10 ³ /uL	22 RDW-CV	15.0	11.0-16.0	%
8 Lym#	2.55	0.80-4.00	10 ³ /uL	23 RDW-SD	46.4	35.0-56.0	fL
9 Mon#	0.87	0.12-1.20	10 ³ /uL	24 PLY	468	100-300	10 ³ /uL
10 Eos#	0.04	0.02-0.50	10 ³ /uL	25 MPV	9.6	6.5-12.0	fL
11 Bas#	0.04	0.00-0.10	10 ³ /uL	26 PCT	0.452	0.108-0.282	%
12 *ALY#	0.04	0.00-0.20	10 ³ /uL	27 P-LCR	23.1	11.0-45.0	%
13 *ALY%	0.5	0.0-2.0	%	28 P-LCC	108	30-90	10 ⁹ /L
14 *LIC#	0.02	0.00-0.20	10 ³ /uL				
15 *LIC%	0.3	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:13

Delivery Time: 2020/06/10 08:13

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 85001309
Run Time: 2020/06/10 08:11
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	10.73 ↑	4.00-10.00	10 ³ /uL	16 RBC	4.93	3.50-5.50	10 ⁶ /uL
2 Neu%	60.5	50.0-70.0	%	17 HGB	11.8	11.0-16.0	g/dL
3 Lym%	29.7	20.0-40.0	%	18 HCT	37.0	37.0-54.0	%
4 Mon%	6.4	3.0-12.0	%	19 MCV	75.1 ↓	80.0-100.0	fL
5 Eos%	3.2	0.5-5.0	%	20 MCH	23.9 ↓	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	31.8 ↓	32.0-36.0	g/dL
7 Neu#	6.48	2.00-7.00	10 ³ /uL	22 RDW-CV	16.5 ↑	11.0-16.0	%
8 Lym#	3.18	0.80-4.00	10 ³ /uL	23 RDW-SD	44.3	35.0-56.0	fL
9 Mon#	0.69	0.12-1.20	10 ³ /uL	24 PLT	391 ↑	100-300	10 ³ /uL
10 Eos#	0.34	0.02-0.50	10 ³ /uL	25 MPV	11.9	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.466 ↑	0.108-0.282	%
12 *ALY#	0.08	0.00-0.20	10 ³ /uL	27 P-LCR	39.4	11.0-45.0	%
13 *ALY%	0.8	0.0-2.0	%	28 P-LCC	154 ↑	30-90	10 ⁹ /L
14 *LIC#	0.05	0.00-0.20	10 ³ /uL				
15 *LIC%	0.5	0.0-2.5	%				

**** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:11

Delivery Time: 2020/06/10 08:11

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:38

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID: 85001304

Sample ID: invalid4
Run Time: 2020/06/10 08:24
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	6.23	4.00-10.00	10 ³ /uL	16 RBC	4.21	3.50-5.50	10 ⁶ /uL
2 Neu%	53.5	50.0-70.0	%	17 HGB	12.5	11.0-16.0	g/dL
3 Lym%	38.8	20.0-40.0	%	18 HCT	37.1	37.0-54.0	%
4 Mon%	7.0	3.0-12.0	%	19 MCV	88.2	80.0-100.0	fL
5 Eos%	0.5	0.5-5.0	%	20 MCH	29.8	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	33.7	32.0-36.0	g/dL
7 Neut#	3.33	2.00-7.00	10 ³ /uL	22 RDW-CV	13.8	11.0-16.0	%
8 Lym#	2.42	0.80-4.00	10 ³ /uL	23 RDW-SD	43.6	35.0-56.0	fL
9 Mon#	0.44	0.12-1.20	10 ³ /uL	24 PLT	172	100-300	10 ³ /uL
10 Eos#	0.03	0.02-0.50	10 ³ /uL	25 MPV	13.1	6.5-12.0	fL
11 Bas#	0.01	0.00-0.10	10 ³ /uL	26 PCT	0.225	0.108-0.282	%
12 *ALY#	0.06	0.00-0.20	10 ³ /uL	27 P-LCR	48.8	11.0-45.0	%
13 *ALY%	1.0	0.0-2.0	%	28 P-LCC	84	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.1	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:24

Delivery Time: 2020/06/10 08:24

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

*The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.

DR. B LAL CLINICAL LABORATORY

First Name:
Last Name:
Gender:
Age:

Sample Type:
Department:
Patient ID:

Sample ID: 96000205
Run Time: 2020/06/10 08:22
Diagnosis:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	5.67	4.00-10.00	10 ³ /uL	16 RBC	4.60	3.50-5.50	10 ⁶ /uL
2 Neu%	47.9 ↓	50.0-70.0	%	17 HGB	14.2	11.0-16.0	g/dL
3 Lym%	39.9	20.0-40.0	%	18 HCT	42.6	37.0-54.0	%
4 Mon%	7.2	3.0-12.0	%	19 MCV	92.6	80.0-100.0	fL
5 Eos%	4.6	0.5-5.0	%	20 MCH	30.8	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	33.3	32.0-36.0	g/dL
7 Neu#	2.72	2.00-7.00	10 ³ /uL	22 RDW-CV	13.3	11.0-16.0	%
8 Lym#	2.26	0.80-4.00	10 ³ /uL	23 RDW-SD	44.1	35.0-56.0	fL
9 Mon#	0.41	0.12-1.20	10 ³ /uL	24 PLT	184	100-300	10 ³ /uL
10 Eos#	0.27	0.02-0.50	10 ³ /uL	25 MPV	15.0 ↑	6.5-12.0	fL
11 Bas#	0.01	0.00-0.10	10 ³ /uL	26 PCT	0.276	0.108-0.262	%
12 *ALY#	0.06	0.00-0.20	10 ³ /uL	27 P-LCR	61.4 ↑	11.0-45.0	%
13 *ALY%	1.1	0.0-2.0	%	28 P-LCC	113 ↑	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:
Description:

Microscopic exam. Time:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:22

Delivery Time: 2020/06/10 08:22

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:

Sample Type:

Sample ID: 96000206

Last Name:

Department:

Run Time: 2020/06/10 08:24

Gender:

Patient ID:

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	11.44 ↑	4.00-10.00	10 ³ /uL	16 RBC	4.54	3.50-5.50	10 ⁶ /uL
2 Neu%	71.1 ↑	50.0-70.0	%	17 HGB	13.6	11.0-16.0	g/dL
3 Lym%	19.9 ↓	20.0-40.0	%	18 HCT	40.8	37.0-54.0	%
4 Mon%	8.4	3.0-12.0	%	19 MCV	89.9	80.0-100.0	fL
5 Eos%	0.4 ↓	0.5-5.0	%	20 MCH	30.0	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	33.4	32.0-36.0	g/dL
7 Neut#	8.13 ↑	2.00-7.00	10 ³ /uL	22 RDW-CV	15.3	11.0-16.0	%
8 Lym#	2.28	0.80-4.00	10 ³ /uL	23 RDW-SD	48.8	35.0-56.0	fL
9 Mon#	0.96	0.12-1.20	10 ³ /uL	24 PLT	146	100-300	10 ³ /uL
10 Eos#	0.05	0.02-0.50	10 ³ /uL	25 MPV	12.4 ↑	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.181	0.108-0.282	%
12 *ALY#	0.03	0.00-0.20	10 ³ /uL	27 P-LCR	45.0	11.0-45.0	%
13 *ALY%	0.3	0.0-2.0	%	28 P-LCC	66	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:24

Delivery Time: 2020/06/10 08:24

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:

Sample Type:

Sample ID: 85001303

Last Name:

Department:

Run Time: 2020/06/10 08:21

Gender:

Patient ID:

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	8.23	4.00-10.00	10 ³ /uL	16 RBC	3.89	3.50-5.50	10 ⁶ /uL
2 Neu%	55.2	50.0-70.0	%	17 HGB	12.5	11.0-16.0	g/dL
3 Lym%	35.3	20.0-40.0	%	18 HCT	38.1	37.0-54.0	%
4 Mon%	6.7	3.0-12.0	%	19 MCV	97.9	80.0-100.0	fL
5 Eos%	2.6	0.5-5.0	%	20 MCH	32.2	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	32.9	32.0-36.0	g/dL
7 Neu#	4.54	2.00-7.00	10 ³ /uL	22 RDW-CV	16.8	11.0-16.0	%
8 Lym#	2.91	0.80-4.00	10 ³ /uL	23 RDW-SD	58.9	35.0-56.0	fL
9 Mon#	0.55	0.12-1.20	10 ³ /uL	24 PLT	128	100-300	10 ³ /uL
10 Eos#	0.21	0.02-0.50	10 ³ /uL	25 MPV	13.2	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.168	0.108-0.282	%
12*ALY#	0.09	0.00-0.20	10 ³ /uL	27 P-LCR	46.6	11.0-45.0	%
13*ALY%	1.0	0.0-2.0	%	28 P-LCC	62	30-90	10 ⁹ /L
14*LIC#	0.00	0.00-0.20	10 ³ /uL				
15*LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:21

Delivery Time: 2020/06/10 08:21

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

DR. B LAL CLINICAL LABORATORY

First Name:

Sample Type:

Sample ID: 85001317

Last Name:

Department:

Run Time: 2020/06/10 08:15

Gender:

Patient ID:

Diagnosis:

Age:

Parameter	Result	Ref. Range	Unit	Parameter	Result	Ref. Range	Unit
1 WBC	10.27 ↑	4.00-10.00	10 ³ /uL	16 RBC	4.71	3.50-5.50	10 ⁶ /uL
2 Neu%	65.1	50.0-70.0	%	17 HGB	11.6	11.0-16.0	g/dL
3 Lym%	29.2	20.0-40.0	%	18 HCT	35.3 ↓	37.0-54.0	%
4 Mon%	4.9	3.0-12.0	%	19 MCV	75.0 ↓	80.0-100.0	fL
5 Eos%	0.6	0.5-5.0	%	20 MCH	24.7 ↓	27.0-34.0	pg
6 Bas%	0.2	0.0-1.0	%	21 MCHC	32.9	32.0-36.0	g/dL
7 Neu#	6.69	2.00-7.00	10 ³ /uL	22 RDW-CV	16.8 ↑	11.0-16.0	%
8 Lym#	3.00	0.80-4.00	10 ³ /uL	23 RDW-SD	44.9	35.0-56.0	fL
9 Mon#	0.50	0.12-1.20	10 ³ /uL	24 PLT	306 ↑	100-300	10 ³ /uL
10 Eos#	0.06	0.02-0.50	10 ³ /uL	25 MPV	12.7 ↑	6.5-12.0	fL
11 Bas#	0.02	0.00-0.10	10 ³ /uL	26 PCT	0.390 ↑	0.108-0.282	%
12 *ALY#	0.08	0.00-0.20	10 ³ /uL	27 P-LCR	45.2 ↑	11.0-45.0	%
13 *ALY%	0.7	0.0-2.0	%	28 P-LCC	138 ↑	30-90	10 ⁹ /L
14 *LIC#	0.00	0.00-0.20	10 ³ /uL				
15 *LIC%	0.0	0.0-2.5	%				

*** means "Research use only, not for diagnostic use".

Sample Type:

Microscopic exam. Time:

Description:

Submitter:

Operator: admin

Approver: service

Sampling Time: 2020/06/10 08:15

Delivery Time: 2020/06/10 08:15

Validated Time: 2020/06/10 08:38

Report Time: 2020/06/10 08:37

Remarks:

***The Report is responsible for this sample only. If you have any questions, please contact us in 24 hours.**

KAWA

DEKORATOR

18/10/2018

18/10/18

 Blood Sample 1 Blood Sample 2 Blood Sample 3 Blood Sample 4 Blood Sample 5

PKM	SQC	SLC	SLB	SLC	PL
Target	0.24	0.27	0.25	0.13	0.04
1	0.05	0.20	0.24	0.14	0.04
2	0.00	0.35	0.14	0.16	0.02
3	0.06	0.24	0.18	0.17	0.13
4	0.00	0.20	0.16	0.16	0.07
5	0.02	0.48	0.18	0.18	0.04
6	0.00	0.00	0.15	0.18	0.00
7	0.09	0.20	0.15	0.14	0.04
8	0.04	0.20	0.15	0.16	0.07
9	0.00	0.07	0.12	0.15	0.00
10	0.00	0.21	0.14	0.16	0.04
Mean	0.023	0.207	0.164	0.166	0.013
SD	0.1	0.1	0.0	0.0	0.0
U.P. (Upper Control Limit)	0.030	0.220	0.170	0.170	0.010

Precision data



Customer Name:	DR B.LAL CLINICAL LABORATORY PVT LTD
Address:	SIKAR

IBM Analyser	ELITE 180
Analyser Sr. No.:	K11051502010
Installation Date:	10 Jun 20
S/W Version	
Study Name	Simple Recursion


Doctor/ HOD Name:	
Engineer Name:	KRISHESH DESHWAL
Application Spl. Name:	Antich (uri)

Sheet Name	Parameters	Sample Id.	Primary Run Value	Units	Primary Run Date & Time	Study start Date & Time	Mean	S.D	CV%
Parameter-1	WBC	85002150.000	8.950	10 ⁹ /L	7/1/2020 10:00	7/1/2020 12:00	9.78	0.23	2.31%
Parameter-2	RBC	85002150.000	5.71	10 ¹² /L	7/1/2020 10:00	7/1/2020 12:00	3.740	0.019416408	0.00502
Parameter-3	HGB	85002150.000	11.1	G/DL	7/1/2020 10:00	7/1/2020 12:00	10.98	0.083666003	0.00762
Parameter-4	PLT	85002150.000	347	10 ⁹ /L	7/1/2020 10:00	7/1/2020 12:00	360.4	6.790527408	0.018605
Parameter-5	HCT	85002150.000	30.1	%	7/1/2020 10:00	7/1/2020 12:00	31.28	0.2105	0.66
Parameter-6	HCT	85002150.000	30.1	%	7/1/2020 10:00	7/1/2020 12:00	31.28	0.2105	0.66
Parameter-7									



Abhishek
Sharma

Sample ID	85002150
Parameter	WBC
Primary Sample Run Parameter Value	8.95
Units of Reporting	10 ³ /UL
Primary Sample Run Date & Time (Analyzer Processing Date & Time) from Raw Data	1-Jul-20
Sample ID Input for Retention Study	85002150
Start Date & Time of Study (Analyzer Processing Date & Time) from Raw Data	1/7/2020 @ 12:38 PM

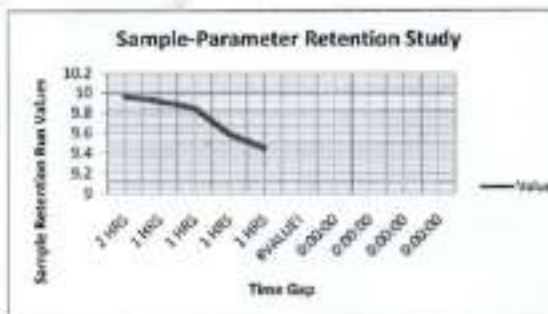


Run #	Date & Time (Analyzer Processing Date & Time) from Raw Data	Time Gap	Value	Difference from Primary Value (B7-Achieved Value)	Variation (within runs)
1	1-7-2020 @ 12:38:00PM	2 HR5	9.97	-1.02	0
2	1-7-2020 @ 13:24PM	1 HR5	9.92	-0.97	0.05
3	1-7-2020 @ 14:23AM	1 HR5	9.85	-0.9	0.07
4	1-7-2020 @ 015:23 PM	1 HR5	9.59	-0.64	0.26
5	1-7-2020 @ 16:45 PM	1 HR5	9.45	-0.5	0.14
6		#VALUE!			
7		0:00:00			0
8		0:00:00			0
9		0:00:00			0
10		0:00:00			



Mean	9.76
S.D	0.225
Cv%	2.31%
Min	9.45
Max	9.97
Min Diff	-1.02
Max Diff	-0.5

Amr

Sample Id.	85002150
Parameter	KAC
Primary Sample Run Parameter Value	3.71
Units of Reporting	10 ⁶ /L
Primary Sample Run Date & Time (Analyzer Processing Date & Time) from Raw Data	1-Jul-20
Sample Id. Input for Retention Study	85002150
Start Date & Time of Study (Analyzer Processing Date & Time) from Raw Data	1-JULY 23 & 12:01 AM

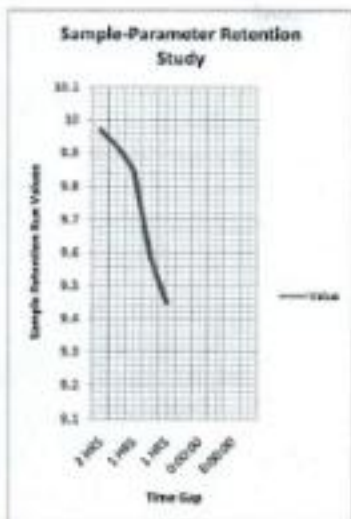


Run #	Date & Time (Analyzer Processing Date & Time) from Raw Data	Time Gap	Value	Difference from Primary Value (RT-Achieved Value)	Variation (within run)
1	1-7-2020 & 12:18:00P M	2 HRS	3.75	-0.02	0
2	1-7-2020 & 12:24PM	1 HRS	3.76	-0.05	-0.03
3	1-7-2020 & 14:23AM	1 HRS	3.76	-0.05	0
4	1-7-2020 & 015:23 PM	1 HRS	3.74	-0.03	0.02
5	1-7-2020 & 38:49 PM	1 HRS	3.74	-0.03	0
6		#VALUE!			
7		0:00:00			0
8		0:00:00			0
9		0:00:00			0
10		0:00:00			0



Handwritten signature

Mean	3.75
S.D	0.013
CV%	0.36%
Min	3.71
Max	3.76
Min Diff	-0.05

Sample ID Input for Retention Study	85002150
PARAMETER	RLT
PRIMARY VALUE	347
UNIT	30°3/UL
Primary Sample Run Date & Time (Analyzer Processing Date & Time) from Raw Data	1-14-20
Sample ID Input for Retention Study	85002150
Start Date & Time of Study (Analyzer Processing Date & Time) from Raw Data	7/2/2020 12:00

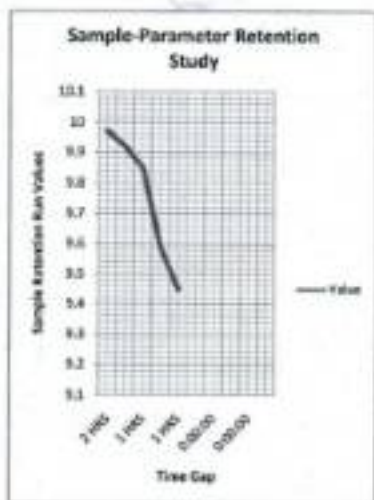


Run #	Date & Time (Analyzer Processing Date & Time) from Raw Data	Time Gap	Value	Difference from Primary Value (IX-Achieved Value)	Variance (with runs)
1	1-7-2020 & 12:18:00PM	2 HRS	357	-10	0
2	1-7-2020 & 12:24PM	1 HRS	361	-14	-4
3	1-7-2020 & 14:23AM	1 HRS	372	-25	-11
4	1-7-2020 & 01:23 PM	1 HRS	358	-11	14
5	1-7-2020 & 16:49 PM	1 HRS	355	-8	3
6		#VALUE!			
7		0:00:00			0
8		0:00:00			0
9		0:00:00			0
10		0:00:00			0



Mean	360.80
S.D	6.731
CV%	1.87%
Min	355
Max	372
Min Diff	-25
Max Diff	-8

Amul

Sample Id. Input for Retention Study	85002150
PARAMETER	HCT
PRIMARY VALUE	30.1
UNIT	%
Primary Sample Run Date & Time (Analyzer Processing Date & Time) from Raw Data	1-Jul-20
Sample Id. Input for Retention Study	85002150
Start Date & Time of Study (Analyzer Processing Date & Time) from Raw Data	7/1/2020 12:00

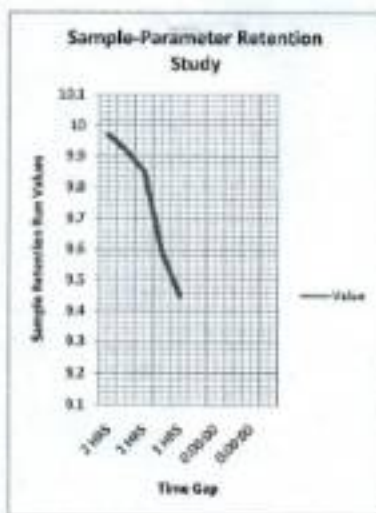

Run #	Date & Time (Analyzer Processing Date & Time) from Raw Data	Time Gap	Value	Difference from Primary Value (RT-Achieved Value)	Variation (within runs)
1	1-7-2020 & 12:18:00PM	1 HRS	31.1	1	0
2	1-7-2020 & 11:24PM	1 HRS	31.5	1.4	-0.4
3	1-7-2020 & 14:23AM	1 HRS	31.5	1.4	0
4	1-7-2020 & 03:23 PM	1 HRS	31.1	1	0.4
5	1-7-2020 & 16:49 PM	1 HRS	31.2	1.1	-0.1
6		#VALUE!			
7		0:00:00			0
8		0:00:00			0
9		0:00:00			0
10		0:00:00			0

Mean	31.28
S.D	0.205
CV%	0.66%
Min	31.1
Max	31.5

Min Diff	1
Max Diff	1.4



Amal