



CERTIFICATE OF CALIBRATION/ VERIFICATION

Customer Name: Agilus Diagnostic Vashi, NAVI MUMBAI.

Model: Fully Automated Bio-Chemistry Analyser-EM 200

Serial No: v200958

Calibration Date: 04-9-2023

Next Calibration due on before : 03-9-2024

Calibrator Used: Multical Lot Number: 230106 Exp 5-10-2023

Quality Control Used: Biorad (L1 89701 & L289702) exp 31-5-2024.

This is to certify that the above mentioned instrument has been verified of calibration according to the procedures provided by the manufacturer -

General Parameters:

Parameter	Measured Value	Acceptable Range	
Line Voltage	230V	230 v +/-	Pass
Logic Voltage	5.0 v	4.9V to 5.1 V	Pass
Lamp Voltage	12.0 v	11.8 V to 12.2 V	Pass
Flow cell Temperature	37.0 deg	37 +/- 0.5	Pass
45 Cuvette blank value for for all filter	Enclose valuesheet for all cuvette	Abs 0.02-0.2	Pass

transasia^{co}.in
www. 

Transasia Ltd., Transasia House, 8 Chandivafi Studio Road, Andheri (East), Mumbai • 400 072
Tel: +91 4030 9000 Fax: +91 22 2857 3030 Email: transasia@transasia.co.in CIN : U33110MH1985PLC036198



Photometer Filter Gain Levels:

s.no	Filter Value in nm	Filter Gain in mv	Acceptable Range of gain
	340	578	50 mv to 200 mv
	405	517	50 mv to 200 rnv
	505	528	50 mv to 200 mv
	546	516	50 mv to 200 mv
	578	495	50 mv to 200 mv
	600	498	50 mv to 200 mv
	660	478	50 mv to 200 mv
	700	460	50 mv to 200 mv

The Results Obtained are as per specifications & tolerance ranges. The above calibration was done with an M/s. Mastech Digital Multimeter.(Model no MAS830L).Sr H62B-D14698.

Technical Service Department

Transasia Bio-medical Limited

Mr. Suraj Chandak
mm-6




CALIBRATION CERTIFICATE

Godrej | CALIBRATION SERVICES

Godrej & Boyce Mfg. Co. Ltd.,
Calibration Services, Plant 18 B, 1st Floor,
Pirojshanagar, Vikhroli,
Mumbai - 400079.
Dr.: +91-22-67965914-48

FR-QT-21	ULR No.:	CC263423000040881F	
Certificate No. : M-231004-21-1	Date of Issue	: 17-Nov-23	
Date of Calibration : 04-Oct-23	Recom. Due Date	: 04-Oct-24	
Customer Details :		Calibrated at	: Lab
Transasia Bio-Medicals Ltd.		Date of Receipt	: 04-Oct-23
Transasia House-8,		Cond. On Receipt	: Satisfactory
Chandivali Studio Road,		Receipt No.	: M-231004-21
Andheri , Mumbai			
Maharashtra India 400072.			
Details of Under Calibration instrument			
Name	: Digital Multimeter	Range	: As Per Report
Make	: Mastech	Sr. No.	: H62B-D14698 ✓
L.C.	: As Per Report	Model	: MAS830L
Details of Master Equipment			
Name	ID No./Sr. No.	Valid Upto	Traceability
Calibration System(9100)	LQE040/924053258	01-Sep-24	Godrej & Boyce, Mumbai
Work Instruction No. :	WI-ET-03		
Environmental Details :	Temperature : 24.5°C	Relative Humidity : 56%RH	
REMARK :			
1. Calibration Points are taken as per Customer's Request.			
2. Group : Electro-Technical, Discipline : Direct Current, Alternating Current < 1 GHz.			
AUTHORIZED SIGNATORY : Asmita Parab			
DESIGNATION : Sr. Calibration Officer			
CALIBRATED BY : Lab Engineer : Rohit Sharma			



Digitally signed by TSD (M) GODREJ AND BOYCE MFG CO LTD
Date: 2023.11.17 16:28:16 +05:30
Reason: Calibration Certificate
Location: Mumbai

Godrej

Godrej & Boyce Mfg. Co. Ltd.

Regd. Office: Pirojshanagar, L.B.S. Marg, Vikhroli, Mumbai - 400 079. T.: +91-22-6796100/1800 W: www.godrej.com
(This document is digitally signed on first page and does not require signature)

TRANSASIA BIO MEDICALS LTD	
TSD Verified By	
Name:	Shilpa Gangan.
Signature:	<i>mg</i>
Date:	18/11/23



CALIBRATION CERTIFICATE

Godrej | CALIBRATION SERVICES
 Godrej & Boyce Mfg. Co. Ltd.,
 Calibration Services, Plant 18 B, 1st Floor,
 Pirojhanagar, Vikhroli,
 Mumbai - 400079.
 Dir.: +91-22-67965914-48

FR-QT-01
 Certificate No.:M-231004-21-1

ULR No.:CC263423000040881F

Range		UUC Reading	Standard Reading	Error in Unit	Measurement Uncertainty (±)(%)	Coverage Factor @ C.L. 95.45 (k)
DC Voltage	200mV	19.9 mV	20.000 mV	-0.100	0.2907	2
		99.4 mV	100.000 mV	-0.600	0.0590	2
		179.2 mV	180.000 mV	-0.800	0.0335	2
		-178.8 mV	-180.000 mV	1.200	0.0335	2
	2V	0.199 V	0.200000 V	-0.001000	0.2889	2
		0.997 V	1.00000 V	-0.00300	0.0590	2
		1.792 V	1.80000 V	-0.00800	0.0335	2
		-1.790 V	-1.80000 V	0.01000	0.0335	2
	20V	1.98 V	2.00000 V	-0.02000	0.2889	2
		9.94 V	10.0000 V	-0.0600	0.0591	2
		17.90 V	18.0000 V	-0.1000	0.0337	2
		-17.88 V	-18.0000 V	0.1200	0.0337	2
	200V	19.8 V	20.0000 V	-0.2000	0.2889	2
		99.5 V	100.000 V	-0.500	0.0592	2
		179.2 V	180.000 V	-0.800	0.0338	2
	600V	-178.9 V	-180.000 V	1.100	0.0338	2
		60 V	60.000 V	0.000	0.9624	2
		300 V	300.000 V	0.000	0.1927	2
		541 V	540.00 V	1.00	0.1076	2
	AC Voltage	200V @50Hz	-541 V	-540.00 V	-1.00	0.1076
19.4 V			20.0000 V	-0.6000	0.2945	2
98.6 V			100.000 V	-1.400	0.0791	2
200V @1KHz		177.4 V	180.000 V	-2.600	0.0773	2
		176.8 V	180.000 V	-3.200	0.0773	2
600V @50Hz		60 V	60.000 V	0.000	0.9641	2
		300 V	300.000 V	0.000	0.2033	2
		540 V	540.00 V	0.00	0.1286	2
600V @1KHz		539 V	540.00 V	-1.00	0.1286	2



Godrej & Boyce Mfg. Co. Ltd.

Regd. Office: Pirojhanagar, L.B.S. Marg, Vikhroli, Mumbai - 400 079. T.:+91-22-67961700/1800 W:www.godrej.com
 (This document is digitally signed on first page and does not require signature)



CALIBRATION CERTIFICATE

Godrej | CALIBRATION SERVICES

Godrej & Boyce Mfg. Co. Ltd.,
 Calibration Services, Plant 18 B, 1st Floor,
 Piroshanagar, Vikhroli,
 Mumbai - 400079.
 Dr.: +91-22-67965914-48

FR-QT-01
 Certificate No.:M-231004-21-1

ULR No.:CC263423000040881F

Range	UUC Reading	Standard Reading	Error in Unit	Measurement Uncertainty (±)(%)	Coverage Factor @ C.L. 95.45 (k)	
Resistance	200Ω	20.8 Ω	20.0000 Ω	0.8000	0.3014	2
		100.2 Ω	100.000 Ω	0.200	0.0740	2
		179.8 Ω	180.000 Ω	-0.200	0.0482	2
	2KΩ	0.199 KΩ	0.200000 KΩ	-0.001000	0.2908	2
		0.914 KΩ	1.00000 KΩ	-0.08600	0.0636	2
		1.741 KΩ	1.80000 KΩ	-0.05900	0.0392	2
	20KΩ	1.98 KΩ	2.00000 KΩ	-0.02000	0.2896	2
		9.97 KΩ	10.0000 KΩ	-0.0300	0.0662	2
		17.94 KΩ	18.0000 KΩ	-0.0600	0.0428	2
	200KΩ	20.1 KΩ	20.0000 KΩ	0.1000	0.2901	2
		99.5 KΩ	100.000 KΩ	-0.500	0.0662	2
		179.1 KΩ	180.000 KΩ	-0.900	0.0428	2
	2MΩ	0.199 MΩ	0.200000 MΩ	-0.001000	0.2901	2
		0.996 MΩ	1.00000 MΩ	-0.00400	0.0902	2
		1.793 MΩ	1.80000 MΩ	-0.00700	0.0718	2
DC Current	200μA	19.9 μA	20.000 μA	-0.100	0.2996	2
		99.6 μA	100.000 μA	-0.400	0.0647	2
		179.2 μA	180.000 μA	-0.800	0.0398	2
		-178.9 μA	-180.000 μA	1.100	0.0398	2
	2mA	0.198 mA	0.200000 mA	-0.002000	0.2896	2
		0.994 mA	1.00000 mA	-0.00600	0.0636	2
		1.790 mA	1.80000 mA	-0.01000	0.0388	2
		-1.788 mA	-1.80000 mA	0.01200	0.0388	2
	20mA	1.98 mA	2.00000 mA	-0.02000	0.2895	2
		9.94 mA	10.0000 mA	-0.0600	0.0637	2
		17.89 mA	18.0000 mA	-0.1100	0.0396	2
		-17.87 mA	-18.0000 mA	0.1300	0.0396	2
	200mA	19.7 mA	20.0000 mA	-0.3000	0.2896	2
		99.4 mA	100.000 mA	-0.600	0.0682	2
		179.0 mA	180.000 mA	-1.000	0.0718	2
10A	-178.8 mA	-180.000 mA	1.200	0.0718	2	
	0.99 A	1.00000 A	-0.01000	0.5863	2	
	4.95 A	5.0000 A	-0.0500	0.1516	2	
	8.94 A	9.0000 A	-0.0600	0.1104	2	
	-8.94 A	-9.0000 A	0.0600	0.1104	2	



Godrej & Boyce Mfg. Co. Ltd.

Regd. Office: Piroshanagar, L.B.S. Marg, Vikhroli, Mumbai - 400 079. T.: +91-22-67961700/1800 W: www.godrej.com
 (This document is digitally signed on first page and does not require signature)



CALIBRATION CERTIFICATE

Godrej | CALIBRATION SERVICES

Godrej & Boyce Mfg. Co. Ltd.,
Calibration Services, Plant 18 B, 1st Floor,
Pirojshanagar, Vikhrol,
Mumbai - 400079
DR.: +91-22-67965814-48

FR-QT-21

Certificate No.:M-231004-21-1

ULR:CC263423000040881F

Remarks:

1. Equipment used for calibration were calibrated & traceable to National & International Standards.
2. This report refers only to particular item (s) submitted for calibration.
3. Godrej Calibration Services is not liable for any change in calibration data & performance specifications on account of malfunctioning of Standards / Instruments / Equipment covered by this report due to damage caused to it after issuance of this report.
4. The calibration results reported are valid at the time of and under the stated conditions of the measurements.
5. The Certificate should not be reproduced except in full without the prior permission from Godrej Calibration Service.
6. Satisfactory calibration report in no ways implies that the equipment calibrated is approved by NABL.
7. All precautions have been taken for any error or omission while calibrating the instruments and issuing this certificate. However Godrej Calibration Services shall not be liable for any loss or liability that may be arise to any party in this regards.
8. Readings given are average of 3 Measurements.
9. The reported Expanded Uncertainty is calculated at 95.45 % Confidence level with coverage factor $k=2$.

— End Of Certificate —

Godrej

Godrej & Boyce Mfg. Co. Ltd.

Regd. Office: Pirojshanagar, L.B.S. Marg, Vikhrol, Mumbai - 400 079.T.:+91-22-67961700/1800 W:www.godrej.com
(This document is digitally signed on first page and does not require signature)

Page 4 of 4

TRACEABILITY

XL MULTICAL

Product Code: XSYS0034

Lot: 2301066

Analyt	Reference Methods / Reference Material	Calibrator value	Uncertainty ¹	Unit
Albumin	CRM 470	3.42	0.043	g/dl
ALP	Original formulation IFCC	300	1.82	U/l
ALT/SGPT	Original formulation IFCC (1985)	89.6	1.25	U/l
AST/SGOT	Original formulation IFCC (1985)	100	0.86	U/l
Amylase	Original formulation IFCC (1998)	186	1.70	U/l
Bilirubin Direct (Walter & Gerarde)	Reference method accor. Jendrassik-Gróf	2.35	0.013	mg/dl
Bilirubin Direct (DCA)	Reference method accor. Jendrassik-Gróf	2.33	0.013	mg/dl
Bilirubin Total (Walter & Gerarde)	Reference method accor. Jendrassik-Gróf	4.95	0.104	mg/dl
Bilirubin Total (DCA)	Reference method accor. Jendrassik-Gróf	4.60	0.096	mg/dl
Calcium	Atomic absorption	10.2	0.063	mg/dl
Chloride	Coulometrie	102	4.73	mmol/l
Cholesterol	ID-MS	170	1.77	mg/dl
CK	Original formulation IFCC (1991)	349	1.91	U/l
CK MB	Original formulation IFCC with immunoinhibition (2002)	408	22.1	U/l
Creatinine (Jaffé)	ID-MS	3.79	0.039	mg/dl
Creatinine (Enz.)	ID-MS	3.79	0.037	mg/dl
GGT	Original formulation Persijn v.d. Slik (1976)	114	1.08	U/l
Glucose	ID-MS	196	1.54	mg/dl
LDH-P	Reference method	491	3.64	U/l
Lipase	Original formulation IFCC	98.9	1.87	U/l
Magnesium	Atomic absorption	2.70	0.021	mg/dl
Phosphorus	Primary reference material	5.52	0.057	mg/dl
Total Protein	SRM 927e	5.10	0.045	g/dl
Triglycerides (single reagent)	SRM 909c	146	1.42	mg/dl
Triglycerides (two reagents)	SRM 909c	147	1.43	mg/dl
Urea	SRM 909c	100	1.04	mg/dl
Uric Acid	ID-MS	5.39	0.034	mg/dl

¹ Expanded uncertainty, $k = 2$

² CRM = Certified reference material, European

³ SRM = Standard reference material

⁴ ID-MS = Isotope dilution – mass spectrometry

Date: 24.04.2023



Dated : 10-4-2024

To,

Agilus Diagnostics

Vashi Navi Mumbai.

Dear Sir,

We Transasia Biomedicals Ltd has Placed Em200 instrument at Agilus Diagnostic vashi with Serial no v200958 is under RR-warranty till 3 Sept2024.

Add: 1st floor Mahavir Centre above golden Punjab hotel sector-17 vashi-400703.

Services Will be continue as Per RR agreement.

Thanks & Regards

A handwritten signature in black ink, appearing to read 'Suraj', is written over a horizontal line.

Suraj Chandak

Area Service Manager.

Transasia Biomedicals Ltd.

Subject : No Equipment Calibration Requirement for FDC 4000i, NX500i and FDC7000i

Design Change Reason	Action	Time frame
<input type="checkbox"/> Specification/Function change <input type="checkbox"/> Pro-active improvement <input type="checkbox"/> Serviceability <input type="checkbox"/> Part Replacement <input type="checkbox"/> Corrective Action <input type="checkbox"/> Preventive Action <input type="checkbox"/> Regulatory Compliance <input checked="" type="checkbox"/> Other (information)	<input type="checkbox"/> Mandatory <input type="checkbox"/> Recommended <input type="checkbox"/> Not required () <input checked="" type="checkbox"/> Other (information only)	<input type="checkbox"/> Immediately <input type="checkbox"/> Next maintenance <input type="checkbox"/> Upon trouble situation <input type="checkbox"/> At your convenience <input checked="" type="checkbox"/> Not Applicable <input type="checkbox"/> Other ()

Date: 06/May/2019 Dept.: Medical Systems Business Div. Originator:

M. Jumawid Edited by: M. Jumawid Approved by: Y. Kashi

Affected Products: FUJI DRI-CHEM analyzers FDC 4000i, NX500i and FDC7000i

To whom it may concern:

This document certifies that FUJI DRI-CHEM analyzers FDC4000i, NX500i and FDC7000i do not require equipment calibration.

The quality of these analyzers is guaranteed through the following principle.

FUJI DRI-CHEM analyzers are equipped with reference white and black plates. The functions of these plates are 1) to adjust the gain for all the interference filters before every measurement, and 2) to assure that the analyzer is working within the manufacturer's quality standard. 2) is conducted after gain adjustment, where the optical densities of reflectance for these plates measured in a constant interval, are checked. If the values exceed the threshold, the machine will indicate an error and the analyzer will not give a measurement result for this abnormal case.

The reference white and black plates are made from ceramic material which do not degrade over time, thus the quality of the analyzers can be confirmed over a long period of time.

- Special tools / Instruments : Yes No

- Supply of the articles : Yes No

If Yes, when :

Name / Code :

- Old parts after replaced : Yes No

- Report requirement after finished : Yes No

TAX INVOICE
(Service Invoice)


000004 8.90

ORIGINAL FOR RECEIPT

Name & Address of Seller: Fujifilm India Pvt Ltd Unitech Cyber Park, 8th Floor, Unit No. 801-807, Tower C Sector -39, Gurugram Postal Code: 122001 Region Code: 06 Haryana GSTIN : 06AABCF159AJZK PAN : AABCF159KJ CIN : U24233DL2007PTC171054	Name & Address of Buyer (Bill To): 1037193 AGILUS PATHLABS PRIVATE LIMITED 12, 1st floor, Above Golden Punjab hotel, Vashi Agilus Pathlabs Vashi, Postal Code: 400703 Region Code: 27 Maharashtra GSTIN: 27AAACT9117E1ZF PAN No. : AAAC91117E	Name & Address of Consignee (Ship To): 1037193 AGILUS PATHLABS PRIVATE LIMITED, Agilus Pathlabs Vashi, 12, 1st floor, Above Golden Punjab hotel, Vashi Contact No: 02262356565 Postal Code : 400703 Region Code : 27 Maharashtra GSTIN : 27AAACT9117E1ZF PAN No. : AAAC91117E
--	--	---

INVOICE NUMBER : 1061764387	Customer Code : 1037193	CARRIER NAME :
DATE : 29.06.2024	PO NO. : 2800003547	VEHICLE NUMBER :
Emergency No. :	PO DATE : 11.06.2024	LR/RN NO. / Date :
Number Of Box : 0	Delivery No. :	Dispatch Through :

SR.	Product Code	HSN/SAC CODE	Product Description	Qty	UOM	Unit Price	Gross Value	Discount	Transaction Value	Rate(%)	IGST		CGST		SGST		
											Amount	Rate(%)	Amount	Rate(%)	Amount	Rate(%)	
1	13400115	998719	AMC-57153227	1,000	AU	30,000.00	30,000.00	0.00	30,000.00	18.00	5,400.00	0.00	0.00	0.00	0.00	0.00	
											Gross Value	30,000.00					
											Total Discount	0.00					
											Advance Payment						
											Taxable Value	30,000.00					
											IGST Total	5,400.00					
											Grand Total	35,400.00					

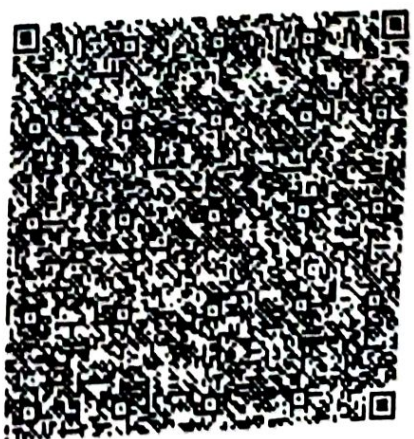

IRN:4b723083c36c4d45d3be79c322571a658896
05a4d5b19d1bf5dc7449396c378d66

Terms of Payment: Due in 90 Days
Please make payment to "FUJIFILM INDIA PVT LTD." HDFC Bank Account No - FUJI401037193. IFSC Code : HDFC0000572
* In Case Of Govt. Customer - " GST TDS should be deducted/deposited as per the supplying State mentioned on INVOICE and Irrespective of PO Location."

General Terms: Goods once sold shall not be taken back. Disputes, if any, shall be subjected to courts of Delhi.
Please receive the undermentioned goods intact per bearer and return the duplicate copy duly signed
In addition to RTGS/NET Online and CHEQUE payments now The FUJIFILM India Pvt. Ltd. is also accepting payments through (i) Debit card (ii) Unified Payments Interface (UPI) (iii) Unified Payments Interface quick response code (UPI QR code) (B-HM UPI QR Code) Machines are available at FUJIFILM Office locations at Kolkata, Chennai, Mumbai & Gurugram for detailed instructions please refer FUJIFILM INDIA Website www.fujifilm.com
Total GST in Words: Five Thousand Four Hundred Rupees Only
Total Invoice Amount in Words: Thirty Five Thousand Four Hundred Rupees Only
Period of contract : 16.06.2024 to 15.06.2025

RECEIVED:
DATE: 03/07/24
SIGN: [Signature]
NAME: Dr. Monika Singh
AGILUS PATHLABS PRIVATE LIMITED
12, 1st floor, Above Golden Punjab hotel, Vashi

FUJIFILM INDIA PVT. LTD.
Authorized Signatory
E & OE
Fujifilm India Pvt Ltd, Reg Office : Business Centre Office No. 621, Level V, Caddle Commercial Tower, Hospitality District Aero city, IGI Airport, New Delhi - 110037
Phone :- 011-66544900 Fax :- 011-66544903 Mail :- contact@fujifilm.com Website :- www.fujifilm.in



FUJIFILM

Value from Innovation

Date: 17 APR 2024

To,
Agilus Pathlabs Private Limited
12, Mahavir Centre, Sector - 17, Vashi,
Sector - 17, Vashi,

Dear Sir/Madam

We thank you for your trust towards Fuji Medical Products and Service Delivery. Hope you have had a good experience with the product and service. In order to continue our best service delivery, we propose the service contract for following equipment's installed at your centre/hospital are as follows.

Equipment	FDC NX 500I
Serial No	57153227
Installation Date	02 MAR 2017
Existing Contract period end date	15 JUN 2024
Customer Code	1037193
Type of Contract	Annual Maintenance Contract
New Contract Period Start-End Date	16 Jun 2024 to 15 Jun 2025
Basic Price Rs.	30000/-
GST Rs. @ 18%	5400/-
Net Value Rs.	35400/-

Terms and Conditions: AMC

1. 100 % advance payment along in favor of FUJIFILM INDIA PRIVATE LIMITED -- RTGS detail- HDFC Bank, Vatika Atrium, A-block, Golf Course Road, Sector-53, Gurugram – 122002, IFSC Code of the Branch - **HDFC0000572**(HDFC Bank), MICR CODE-**110240093**. Account Number **FUJI401037193**
2. 100% payment on basis of **Proforma invoice** and PM report submission.
3. Any failure due to Third party equipment like UPS, batteries or earthing will not be considered as down time of machine.
4. Contract includes 3 preventive maintenance calls. Any number breakdown calls are covered
5. No Labour charges, whereas spares will be on chargeable basis
6. All the Defective replaced spare parts and Good Spare parts to be return back to Fuji warehouse
7. For services under this contract customer can contact Toll Free Number given below or FFIN Engg. Mr. Prabhakar Sharma - 9699258155

Thank You



Ritvik Sen
Regional Service Manager West
Fujifilm India Pvt. Ltd.

Toll free assistance line is now open to you from Mon - Sat (09:00 to 05:30 pm), for better service please log all service complaints @ 1800 103 3854 or email us at medical.services@fujifilm.com

FUJIFILM INDIA PRIVATE LIMITED

Corporate Office : Unitech Cyber Park, 8th floor, Unit no.801-807, Tower C, Sector-39, Gurugram- 122101, Haryana

Telephone : +91-124-4325500, Fax : +91-124-4325555, Website : www.fujifilm.com , Email : Contact@fujifilm.com

Registered Office : Business Centre Office No. 521, Level V, Caddle Commercial Tower, Hospitality District Aerocity IGI Airport, New Delhi-110037, Telephone : +91-11-66544932.

Mumbai Office: Unit No.504 & 505, 5thFloor,349 Business Point, Western Express Highway, Andheri (East), Mumbai-400069
Telephone: +91-22-42364000, Fax +91-22-42364001.

FUJIFILM

Date: 13th July ,2024

Respected Sir/Madam,

Fujifilm NX500I does not required any equipment calibration , However there is a reference card with each box of reagent which has to be scanned in the machine every time there is a change of lot number or a new batch of reagent is put in use. During Periodic maintenance of the machine the optical system including the lamp and the reference pad are checked thoroughly.



Prabhakar Sharma
FUJIFILM INDIA PVT LTD.
(+91 8588870543)

FUJIFILM INDIA PRIVATE LIMITED

Corporate Office: Unitech Cyber Park, Unit No. B01 B07, 8th Floor, Tower C, Sector 35, Gurgaon - 122001, Haryana
Telephone: +91 124 4325500, Fax: +91 124 4325555, Website: www.fujifilm.in
Email: contact@fujifilm.com
CIN: U24233DL2007PTC 171064

Report # 505288

FFIN Copy
TOLL FREE No. 1800-103-3854

FUJIFILM

FUJIFILM India Pvt. Ltd

Unit No. 801-807, 8th Floor, Tower C,
Unitech Cyber Park, Sector 39,
Gurugram-122001, Haryana, INDIA
medical.services@fujifilm.com

Field Service Report

SFDC CASE ID		Date	
		03/05/24	
Customer Details			
Customer Name		Agilus Pathlabs Pvt Ltd	
Address		Ward, Navikumbhari	
State		Maharashtra	
Department		Lab	
Contact Person		Dr. S. Teekchandani	
Phone No.		9029929010	
Email Address			
Equipment's Details			
Equipment Type		FDC	
Model		NX500i	
Serial No.		57153227	
Service Contract Type		<input type="checkbox"/> WARRANTY <input type="checkbox"/> CMC <input checked="" type="checkbox"/> AMC <input type="checkbox"/> PER CALL	
Console Name & Version		Job	
Workstation Name & Version		V3.3	
SR Details			
Call Received Date		08/05/24	
FFIN / Authorized Service Provider		Lifetime Diagnostics Pvt Ltd	
Activity Start Date & time		08/05/24	
Activity End Date & Time		08/05/24	
Total Travel Time (in hrs.)			
Activity Description			
Problem Description / Error		Preventive Maintenance	
Action Taken		checked system and error log done DMG as per the standard procedure Ref plate level = L1 (2g) i. lamp hrs previous = 147h hrs, Now 00 hrs changed lamp of the instrument from customer's stock this sample, control L1 and L2.	
Call Status		<input checked="" type="checkbox"/> COMPLETED <input type="checkbox"/> UNDER OBSERVATION <input type="checkbox"/> INCOMPLETE	
Engineer's Remark (if any)		Instrument is working Satisfactory	
Part Used / Required			
Part Name / Description		Part Code	
LAMP		F1224200002	
Engineer Signature		Customer Remarks	
Riddhe Bagal			
Engineer Name		Customer Signature & Stamp	
Riddhe Bagal		[Signature]	