



Date: 06/01/2024
Effective Date: 06/01/2024

CERTIFICATE OF CALIBRATION

Customer Name : Deepa MRI & Diagnostic Centre


MODEL : EM200

Serial N : V200070

Date of Calibration : 06/01/2024

Next Calibration Due : 05/01/2025

This is to certify that the above mentioned product has been verified of calibration according to the industry standard procedures.

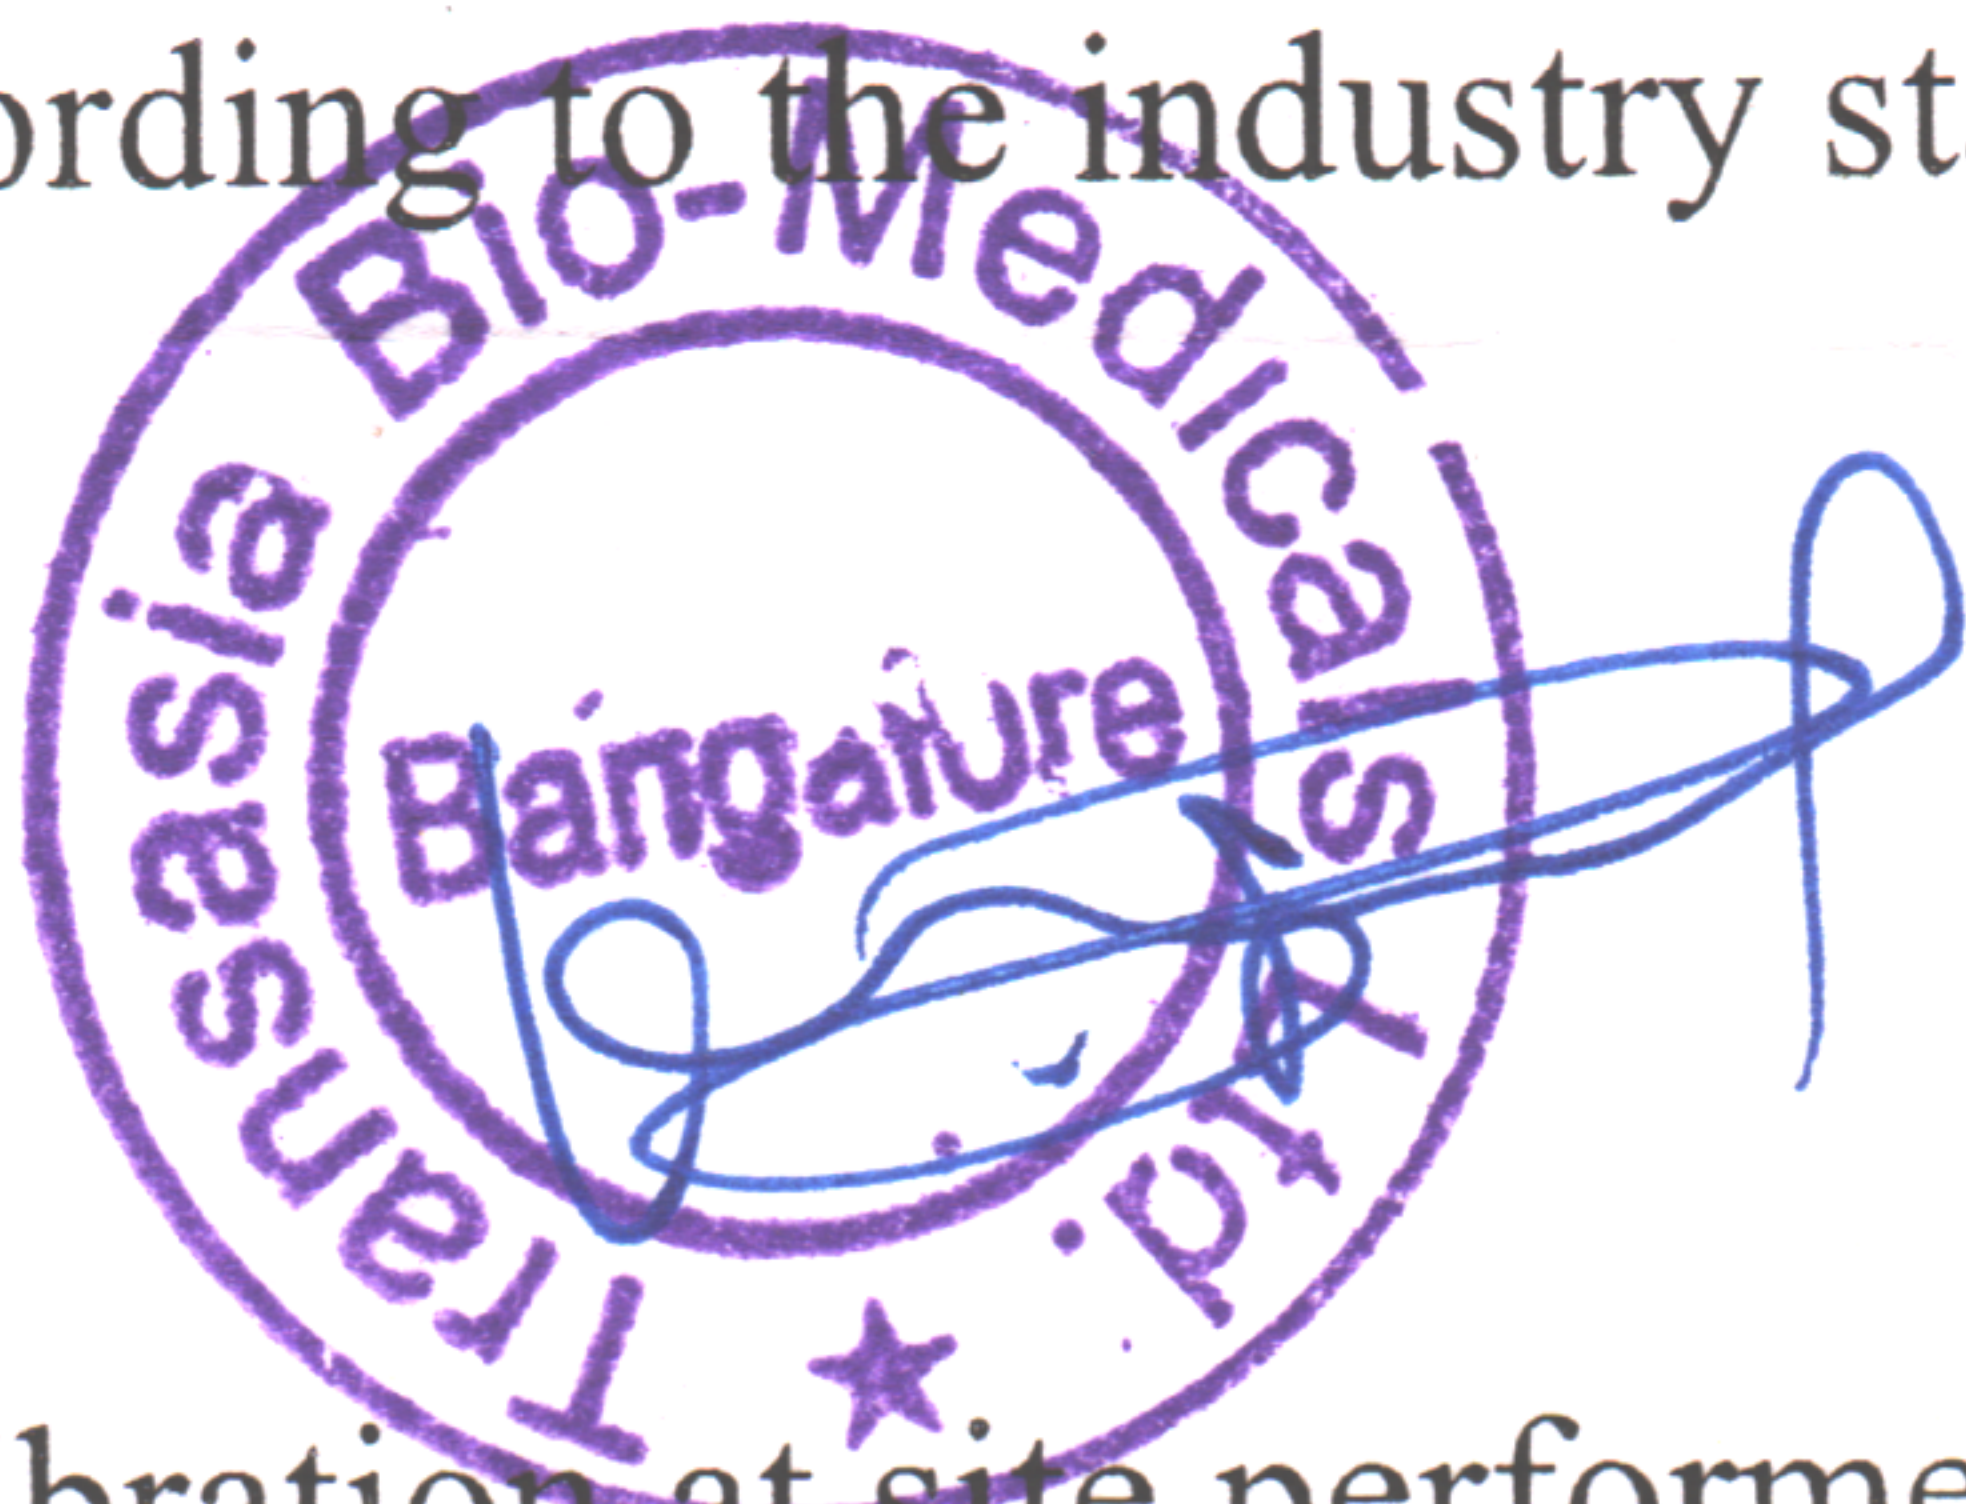

Calibration at site performed by
SRIRAM R

Technical Service Department
Transasia Bio-Medicals Ltd.,
Mumbai.