

CERTIFICATE OF CALIBRATION

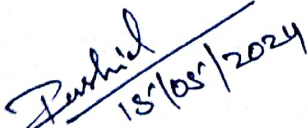
RIB//088/24-25

Customer Name : Ayucare Pathology
Address of the customer : ULWE,NAVI MUMBAI
Instrument Model : H30 Pro 3 Part Hematology Analyzer
Serial No. : 860458-M21908820002
Date of Installation : 20/11/2021
Date of Calibration : 15/05/2024

This is to certify that the above mentioned product has been calibrated for CBC parameters (WBC, RBC, HGB, HCT, PLT) according to the standard operating procedure given by Mindray.

The reference instruments used for value assignment are managed by the traceability system in Agappe diagnostics and these are traceable to the International Standards such as ICSH.

For RIBOSOMES DIAGNOSTICS.


15/05/2024
Authorized Signatory

DETAILS OF CONTROL RUN

Instrument Model : H30 Pro 3 Part Hematology Analyzer
Serial No. : 860458-M21908820002
Date of Control Run : 15/05/2024
Control Used : HEMATOLOGY CONTROL TRI LEVEL
Lot No : 32310038
Expiry : 05/08/2024


The results of repeatability test are summarized in the following table. Refer the attached control sheets for details.

Sample No	WBC K/ μ L	RBC M/ μ L	HGB g/dL	HCT (%)	PLT K/ μ L
1	7.9	4.19	13.2	38.1	245
2	7.8	4.31	13.5	38.7	239
3	8.0	4.25	13.9	38.5	241
Instrument Mean	7.9	4.25	13.5	38.4	241.6
Range	6.9 - 8.6	3.7 - 4.5	12.1 - 13.9	29.4 - 40.4	203 - 275
CV %	1.26 %	1.41 %	2.59 %	0.79 %	1.26 %

This is to certify that the above mentioned product has been calibrated for CBC parameters (WBC, RBC, HGB, HCT, PLT) according to the standard operating procedure given by Mindray.

The control run after calibration shows good repeatability and precision Next Calibration due on 14/05/2025.

For RIBOSOMES DIAGNOSTICS .


15/05/2024
Authorized Signatory