

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024

**Immunoassay Extended, ASO Qualitative, IU/mL**


- All Methods
- Agglutination - (Your Method)
- Manual - (Your Analyzer)

**N**  
68  
18  
32

<b>Your Result</b>	Normal
<b>Result Expected</b>	Nor

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

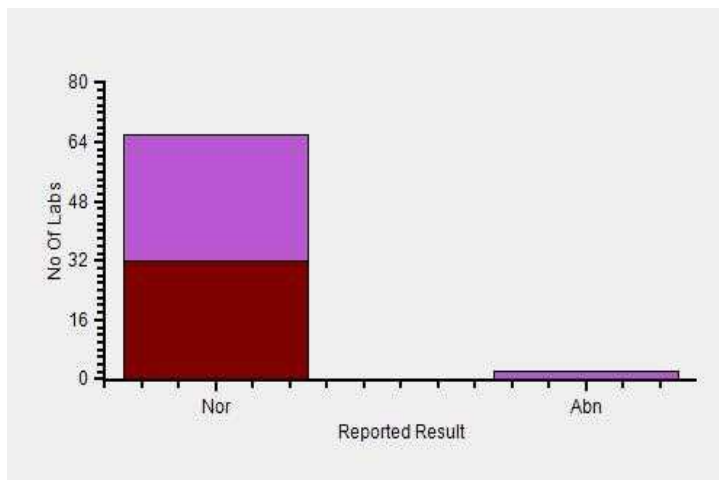

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

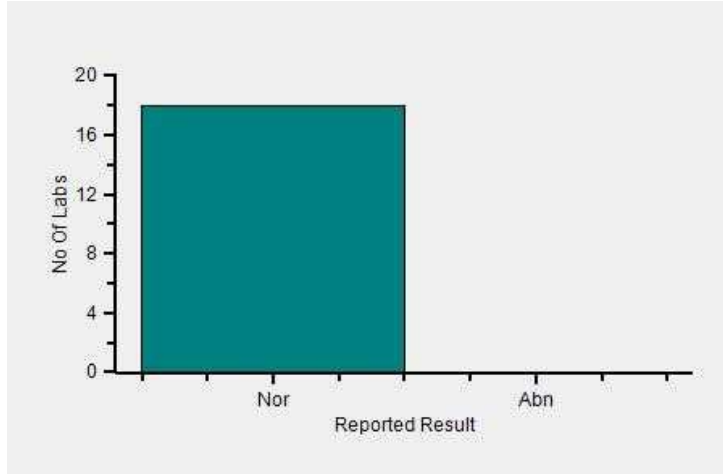

Frequency Histogram Your Analyzer

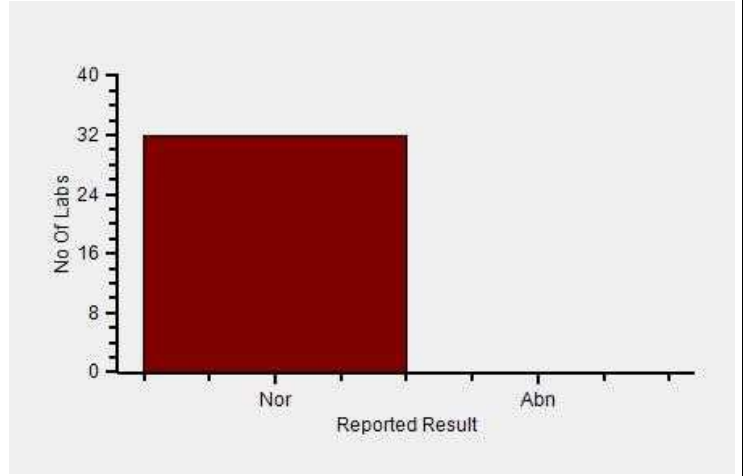

**Reported Results Legends :-**

- Nor** : Normal
- Abn** : Abnormal

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1352  
 Lab Name : TATA 1MG LABS JAIPUR  
 Report Date : 18/10/2024

Cycle No : 240207  
 Sample No : 01  
 Round Open Date : 08/08/2024


**Immunoassay Extended, Dengue IgG, Units**

	<b>N</b>
■ All Methods	193
■ EIA - (Your Method)	18
■ Lisa Scan - (Your Analyzer)	6

<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

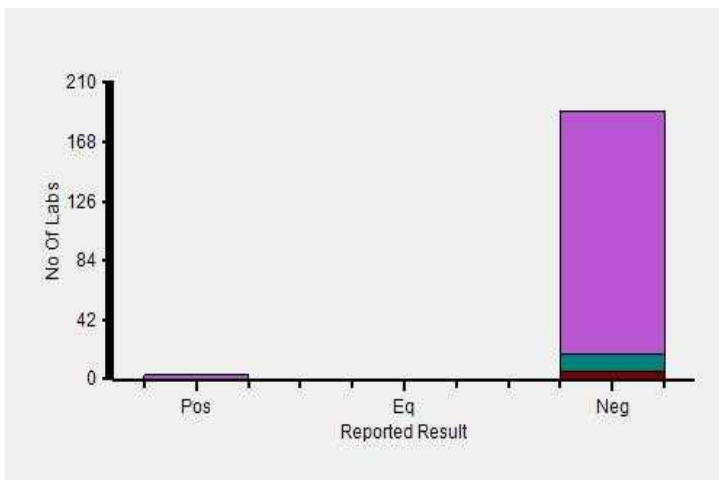

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

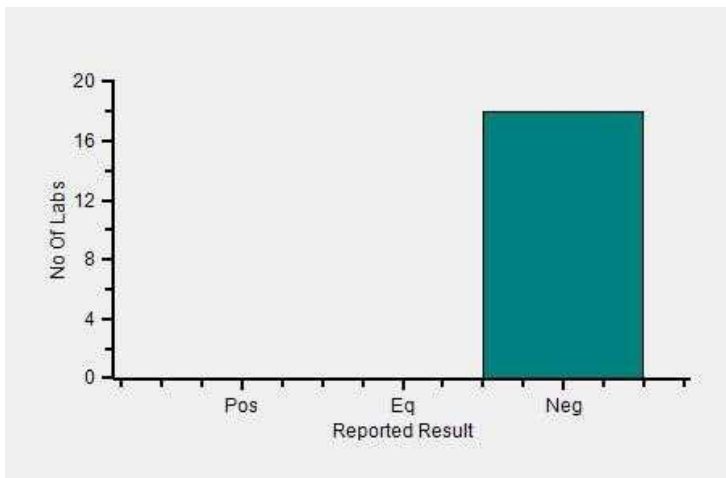

Frequency Histogram Your Analyzer

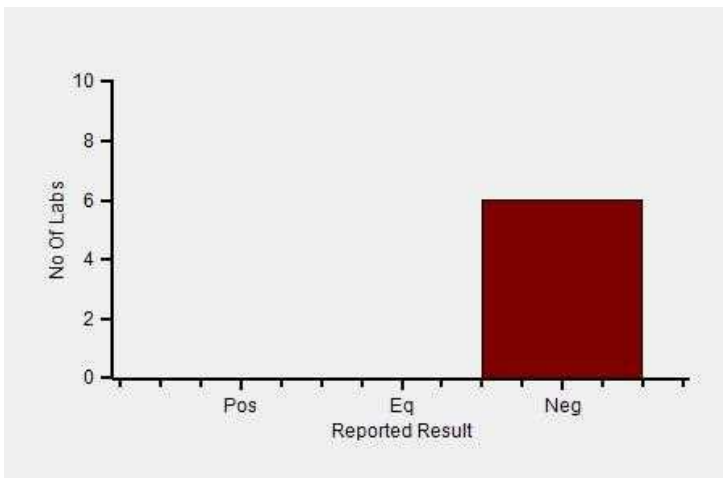

**Reported Results Legends :-**

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1352  
 Lab Name : TATA 1MG LABS JAIPUR  
 Report Date : 18/10/2024

Cycle No : 240207  
 Sample No : 01  
 Round Open Date : 08/08/2024


**Immunoassay Extended, Dengue IgM, Units**

	<b>N</b>
■ All Methods	196
■ EIA - (Your Method)	19
■ Lisa Scan - (Your Analyzer)	7

<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

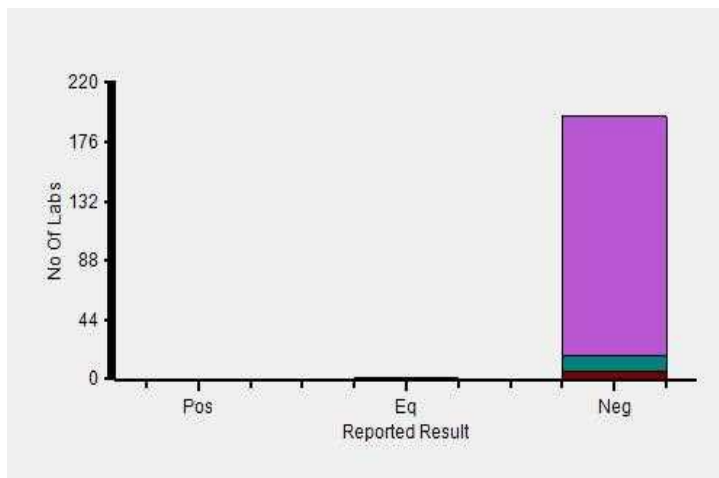

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

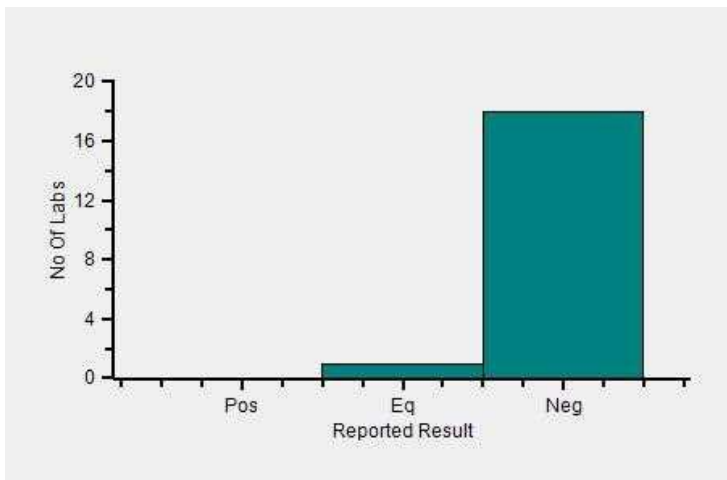

Frequency Histogram Your Analyzer

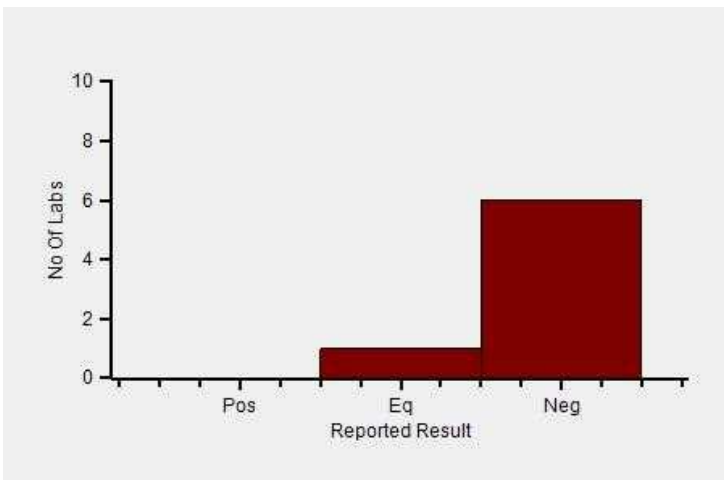

**Reported Results Legends :-**

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024


**Immunoassay Extended, Dengue NS 1, Units**

	<b>N</b>
■ All Methods	259
■ EIA - (Your Method)	25
■ Lisa Scan - (Your Analyzer)	8

<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

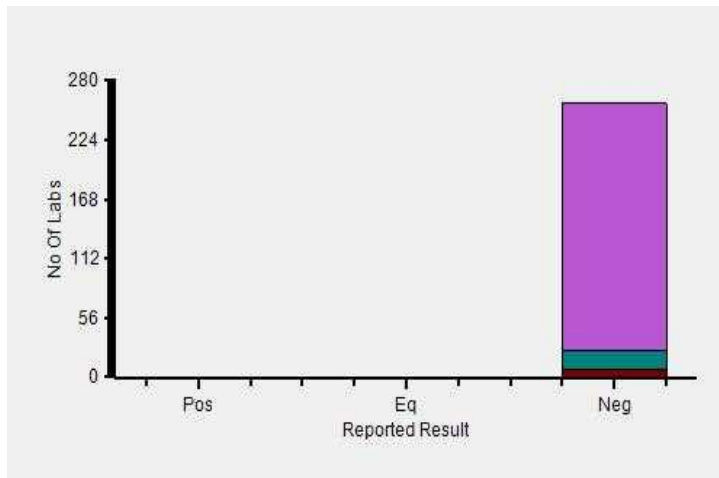

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

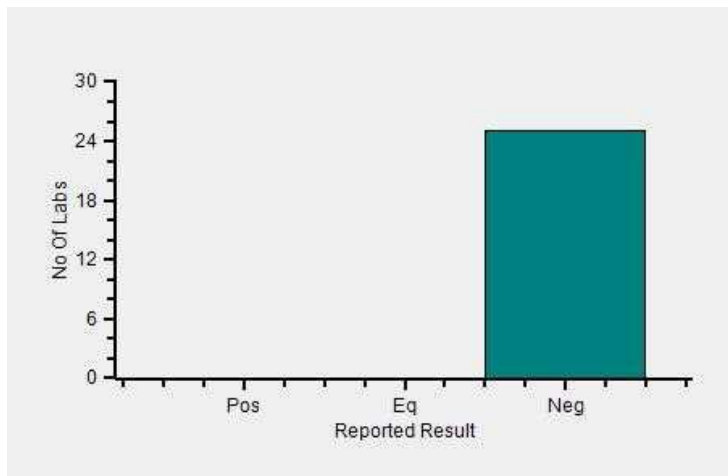

Frequency Histogram Your Analyzer

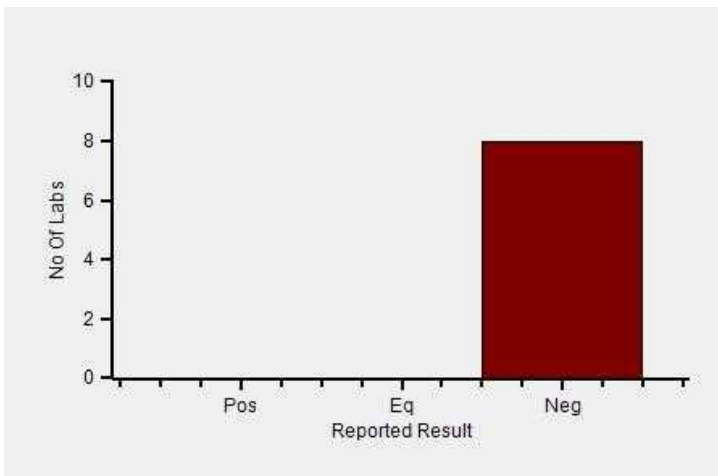

**Reported Results Legends :-**

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error





Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024


**Immunoassay Extended, HBsAg, -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	351
<span style="color: green;">■</span> Immunochromatography - (Your Method)	235
<span style="color: red;">■</span> Manual - (Your Analyzer)	201

<b>Your Result</b>	Non-reactive
<b>Result Expected</b>	NR

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

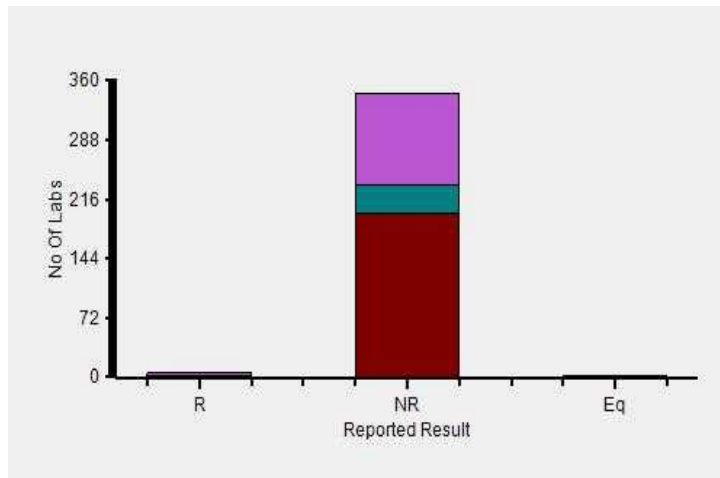

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

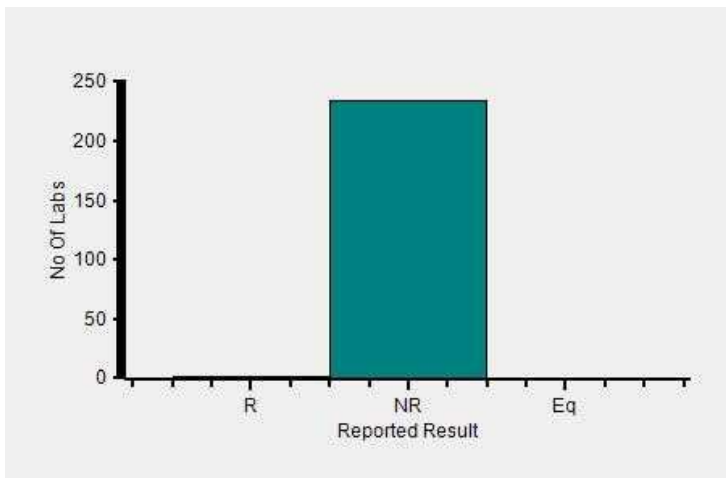

Frequency Histogram Your Analyzer

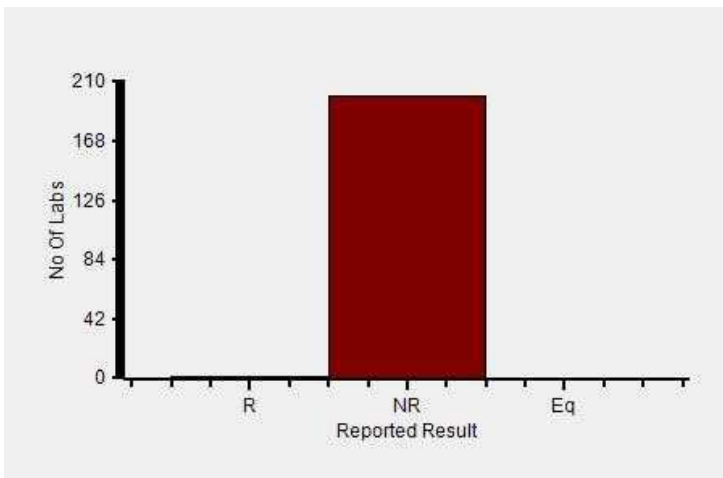

**Reported Results Legends :-**

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1352  
 Lab Name : TATA 1MG LABS JAIPUR  
 Report Date : 18/10/2024

Cycle No : 240207  
 Sample No : 01  
 Round Open Date : 08/08/2024


**Immunoassay Extended, HCV, -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	340
<span style="color: green;">■</span> Immunochromatography - (Your Method)	191
<span style="color: red;">■</span> Manual - (Your Analyzer)	203

<b>Your Result</b>	Non-reactive
<b>Result Expected</b>	NR

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

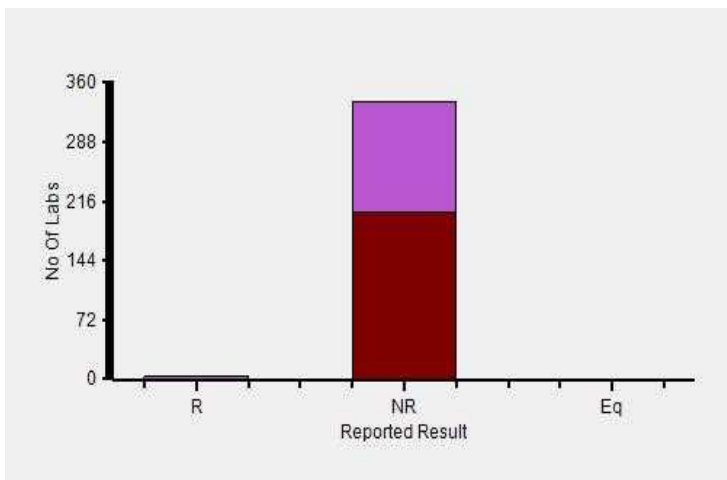

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

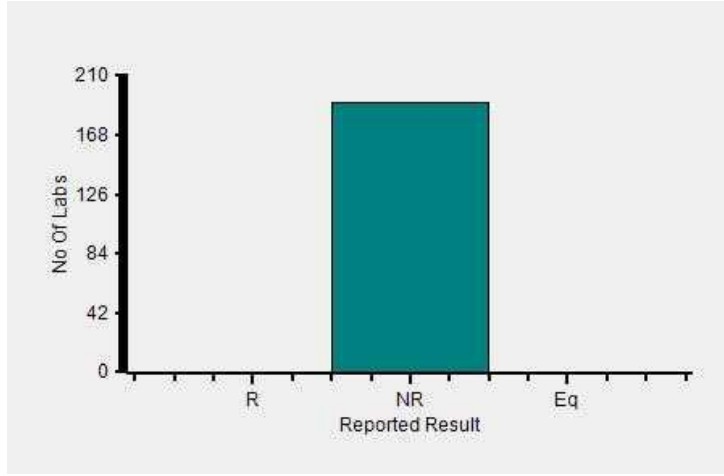

Frequency Histogram Your Analyzer

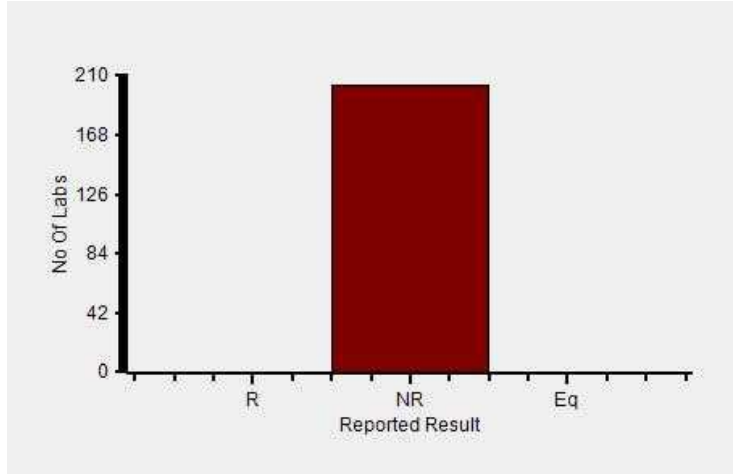

**Reported Results Legends :-**

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1352  
 Lab Name : TATA 1MG LABS JAIPUR  
 Report Date : 18/10/2024

Cycle No : 240207  
 Sample No : 01  
 Round Open Date : 08/08/2024


**Immunoassay Extended, HIV Ab, -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	215
<span style="color: green;">■</span> Immunochromatography - (Your Method)	151
<span style="color: red;">■</span> Manual - (Your Analyzer)	157

<b>Your Result</b>	Non-reactive
<b>Result Expected</b>	NR

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

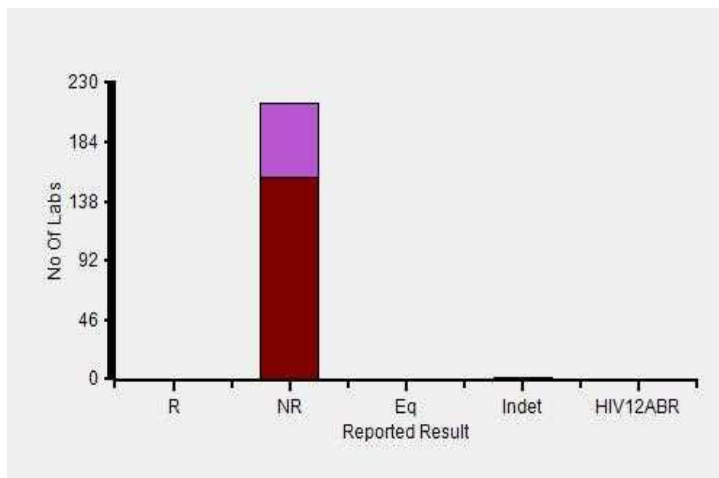

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

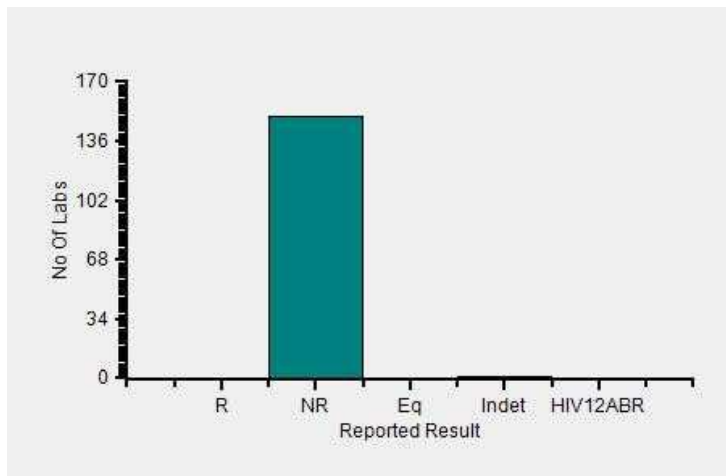

Frequency Histogram Your Analyzer

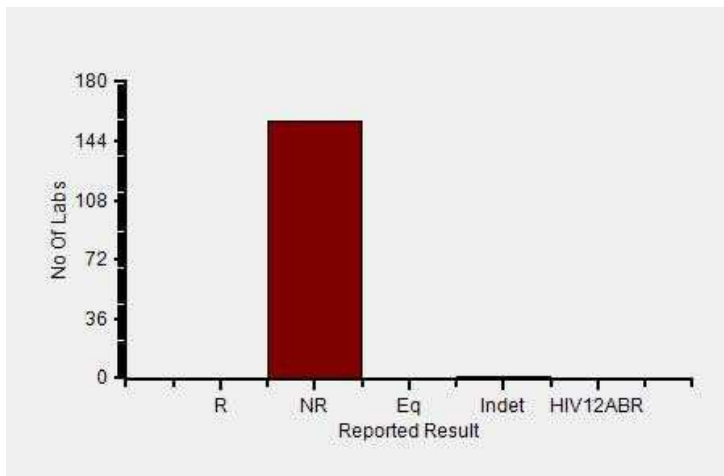

**Reported Results Legends :-**

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal
- Indet** : Indeterminate
- HIV-1** : HIV-1 Ab Reactive
- HIV-2** : HIV-2 Ab Reactive
- HIV12ABR** : HIV-1/HIV-2 Ab Reactive

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024

**Immunoassay Extended, RPR (Syphilis Serology), -**


- All Methods
- Flocculation - (Your Method)
- Manual - (Your Analyzer)

**N**  
 294  
 118  
 294

<b>Your Result</b>	Non-reactive
<b>Result Expected</b>	NR

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

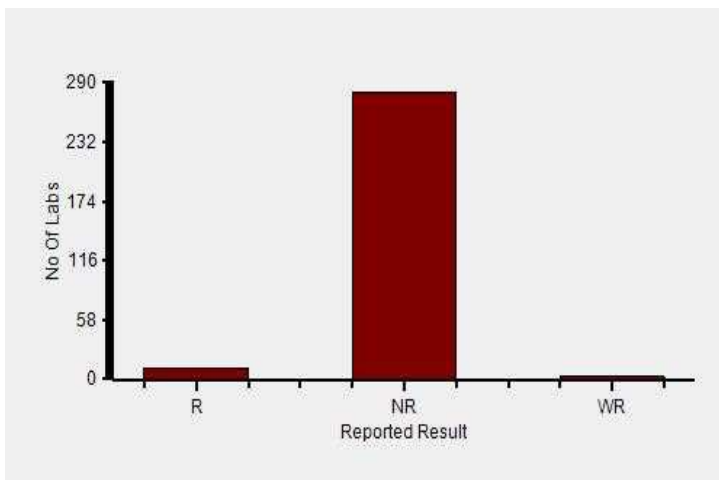

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

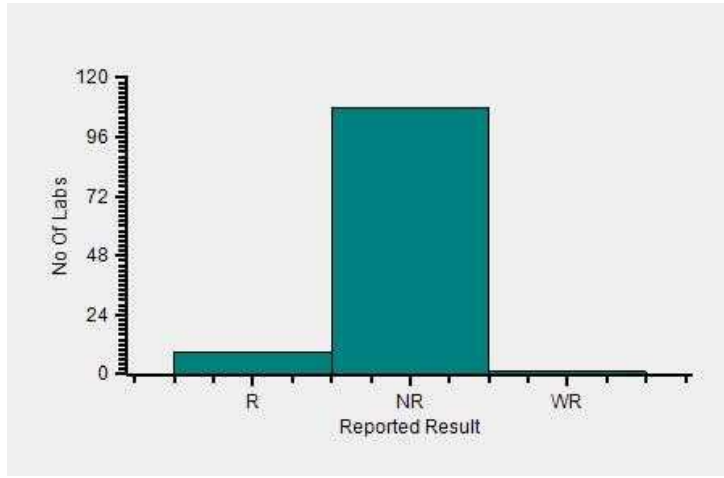

Frequency Histogram Your Analyzer

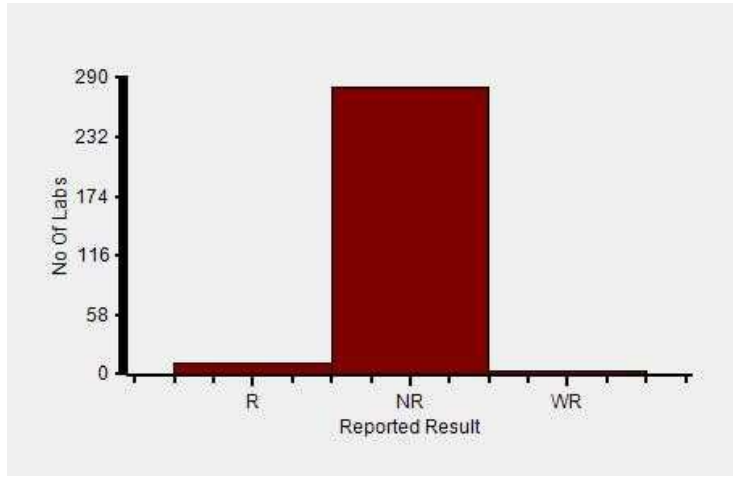

**Reported Results Legends :-**

- R** : Reactive
- NR** : Non-reactive
- WR** : Weak Reactive

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error





Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024


**Immunoassay Extended, Typhidot IgM, -**

	<b>N</b>
■ All Methods	211
■ Immunochromatography - (Your Method)	207
■ Manual - (Your Analyzer)	211

<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

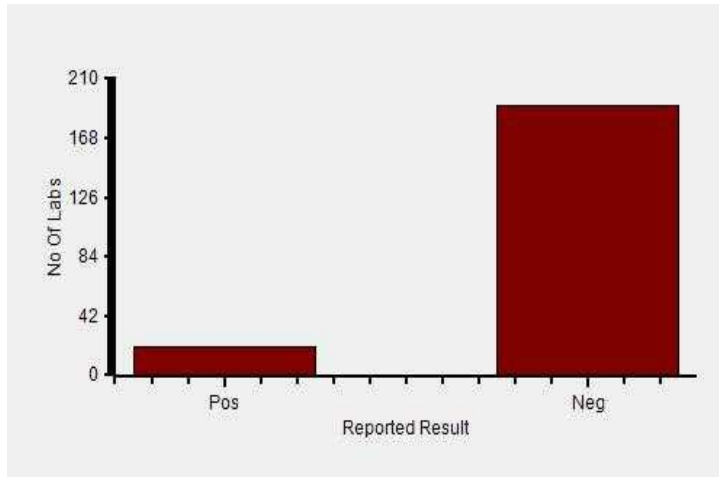

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

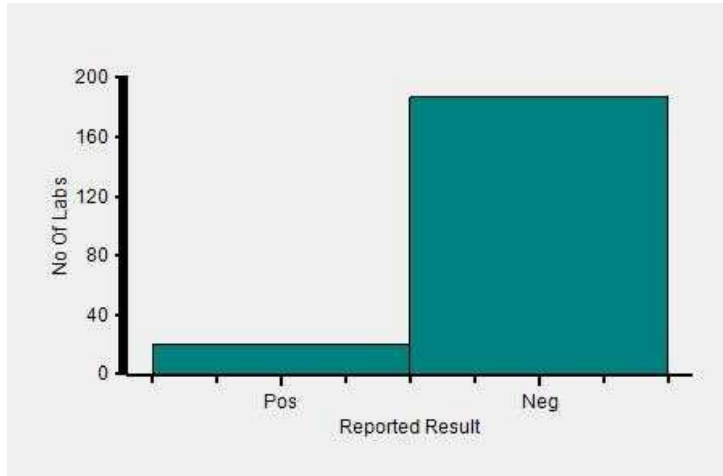

Frequency Histogram Your Analyzer

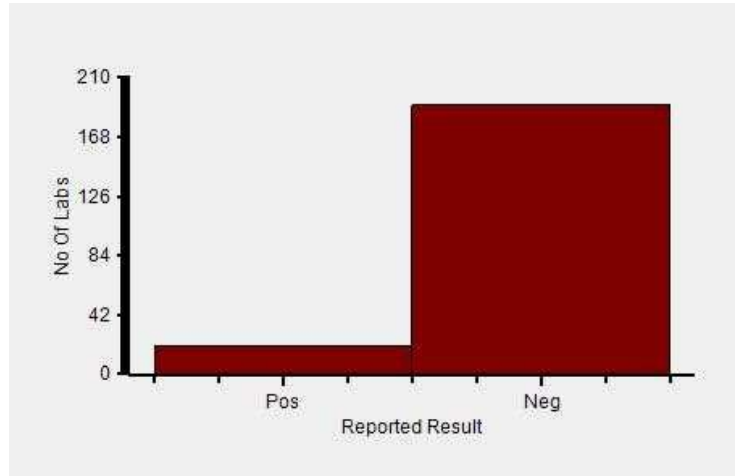

**Reported Results Legends :-**

**Pos** : Positive

**Neg** : Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024


**Immunoassay Extended, Widal test - ParaTyphi A-H antigen (AH), -**

	<b>N</b>
■ All Methods	299
■ Slide Agglutination - (Your Method)	235
■ Manual - (Your Analyzer)	299

<b>Your Result</b>	No Agglutination
<b>Result Expected</b>	NoA

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

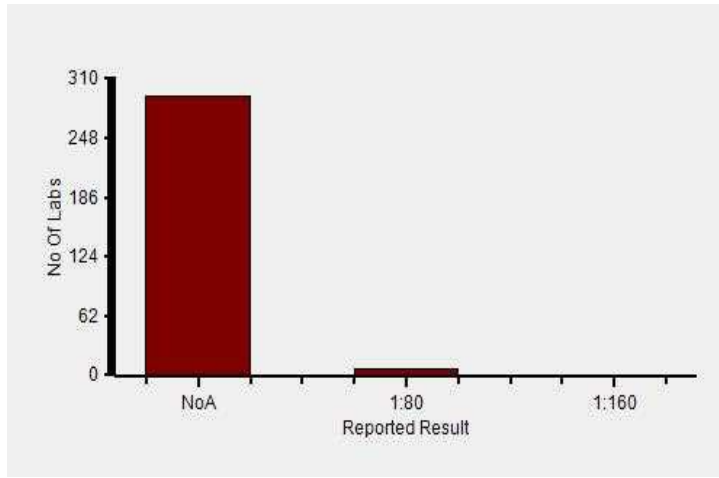

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

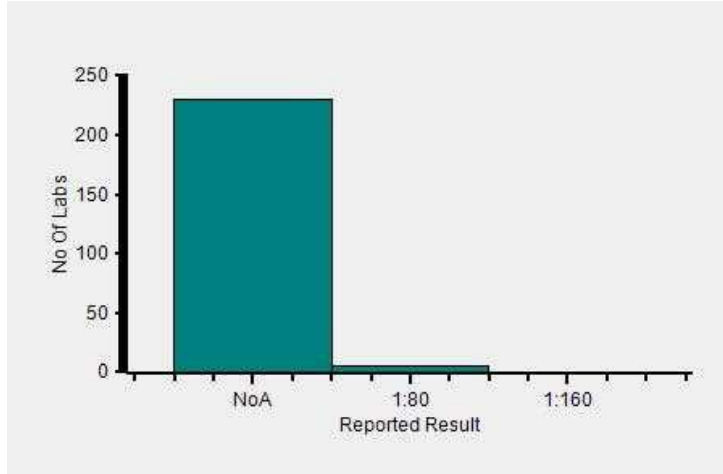

Frequency Histogram Your Analyzer

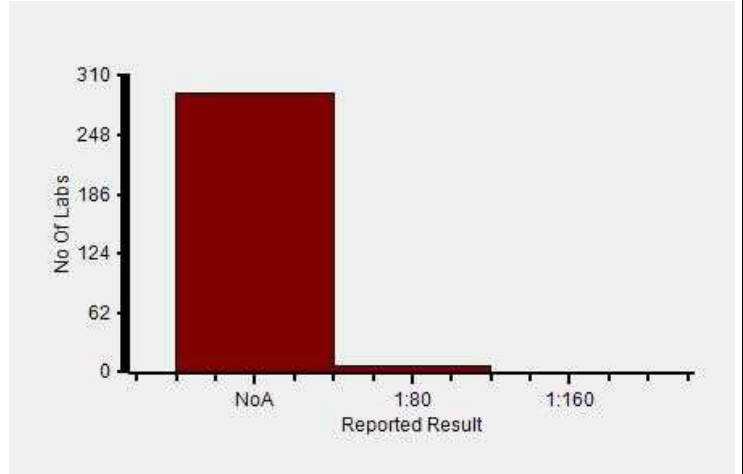

**Reported Results Legends :-**

<b>NoA</b>	: No Agglutination
<b>1:80</b>	: 1:80
<b>1:160</b>	: 1:160
<b>1:320</b>	: 1:320
<b>1:640</b>	: 1:640
<b>&gt;1:640</b>	: >1:640

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- |                       |   |
|-----------------------|---|
| • Two out of two pass | - Acceptable performance                                |
| • One out of two pass | - Review for random error & take action if appropriate  |
| • Both failed         | - Unacceptable performance, Review for systematic error |

b) Reported on 3 samples:

- |                         |   |
|-------------------------|---|
| • All pass              | - Acceptable performance                                |
| • Two out of three pass | - Review for random error & take action if appropriate  |
| • One out of three pass | - Unacceptable performance, Review for systematic error |
| • All failed            | - Unacceptable performance, Review for systematic error |



Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024

**Immunoassay Extended, Widal test - ParaTyphi B-H antigen (BH), -**

■ All Methods

■ Slide Agglutination - (Your Method)

■ Manual - (Your Analyzer)

**N**

298


235

298

<b>Your Result</b>	No Agglutination
<b>Result Expected</b>	NoA

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

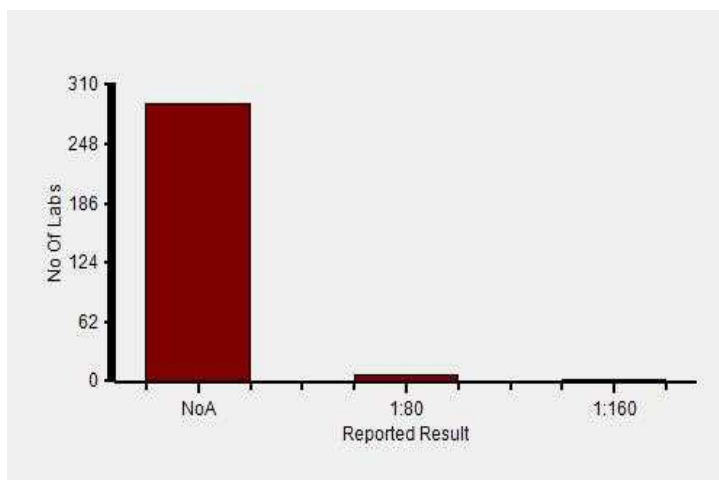

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

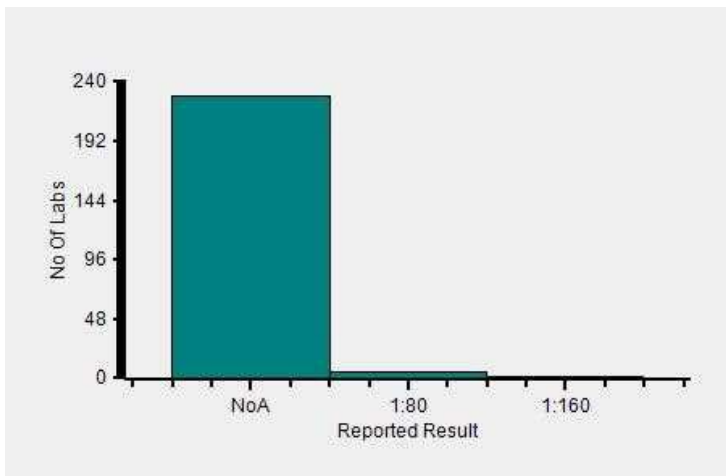

Frequency Histogram Your Analyzer

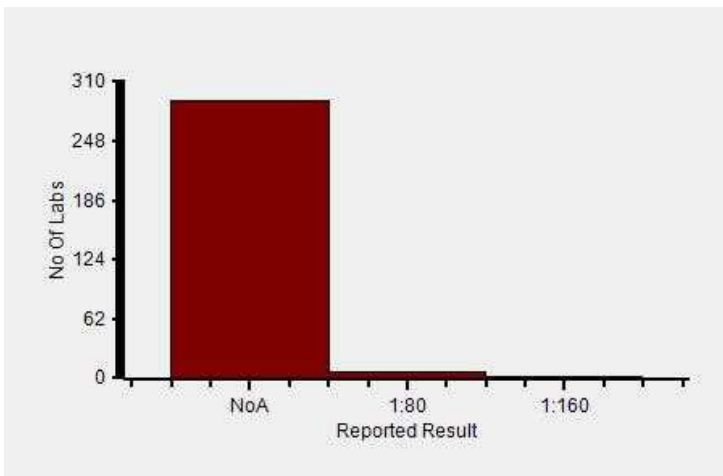

**Reported Results Legends :-**

<b>NoA</b>	: No Agglutination
<b>1:80</b>	: 1:80
<b>1:160</b>	: 1:160
<b>1:320</b>	: 1:320
<b>1:640</b>	: 1:640
<b>&gt;1:640</b>	: >1:640

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1352  
 Lab Name : TATA 1MG LABS JAIPUR  
 Report Date : 18/10/2024

Cycle No : 240207  
 Sample No : 01  
 Round Open Date : 08/08/2024


**Immunoassay Extended, Widal test - Typhi H antigen (TH), -**

	<b>N</b>
■ All Methods	316
■ Slide Agglutination - (Your Method)	251
■ Manual - (Your Analyzer)	316

<b>Your Result</b>	No Agglutination
<b>Result Expected</b>	NoA

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

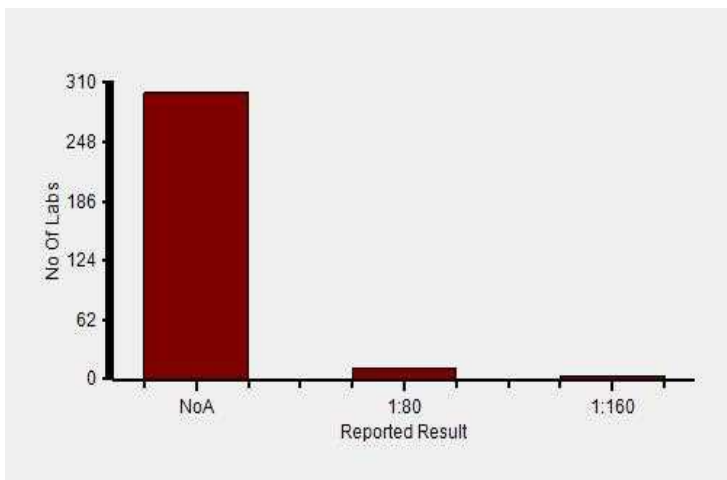

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

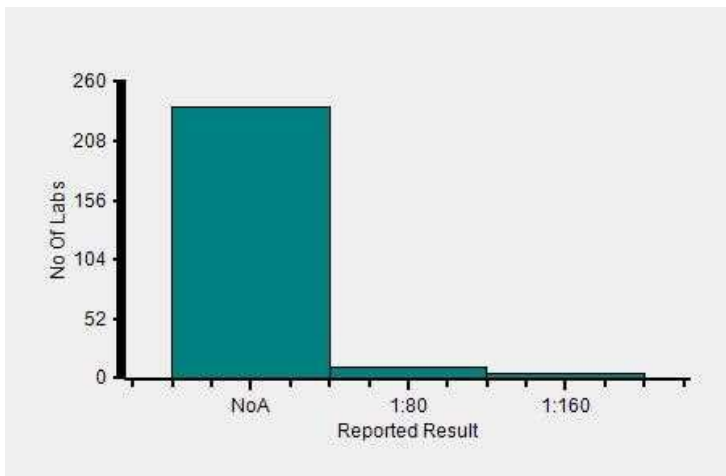

Frequency Histogram Your Analyzer

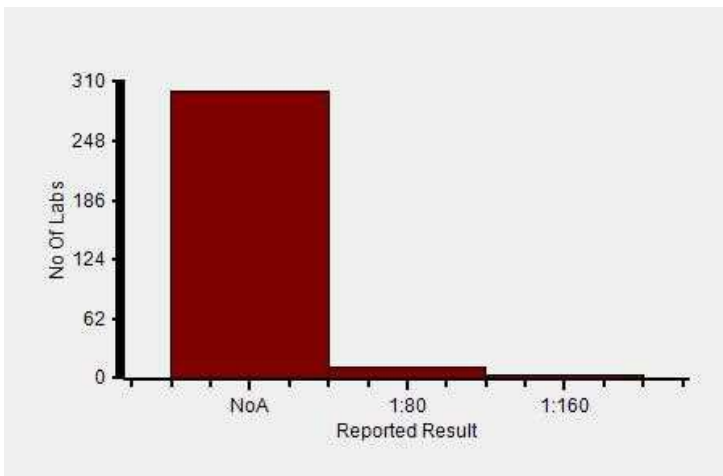

**Reported Results Legends :-**

<b>NoA</b>	: No Agglutination
<b>1:80</b>	: 1:80
<b>1:160</b>	: 1:160
<b>1:320</b>	: 1:320
<b>1:640</b>	: 1:640
<b>&gt;1:640</b>	: >1:640

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error





Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR

Report Date : 18/10/2024

Cycle No : 240207

Sample No : 01

Round Open Date : 08/08/2024

**Immunoassay Extended, Widal test - Typhi O antigen (TO), -**

■ All Methods

■ Slide Agglutination - (Your Method)

■ Manual - (Your Analyzer)

**N**

316


251

316

<b>Your Result</b>	No Agglutination
<b>Result Expected</b>	NoA

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

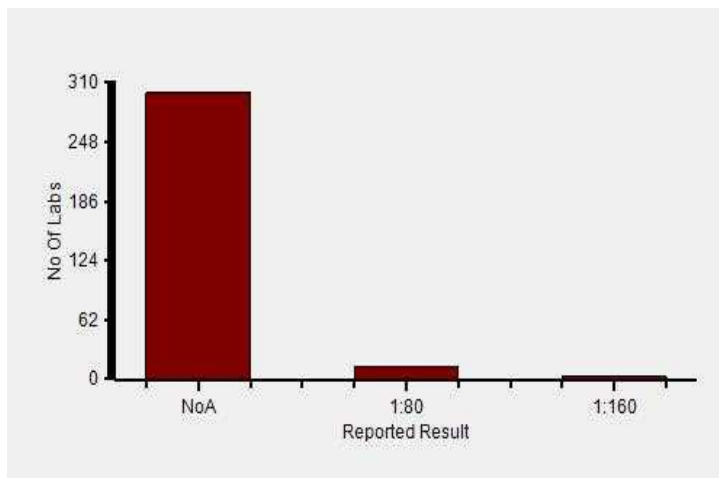

Lab : 1352

Lab Name : TATA 1MG LABS JAIPUR


Report Date : 18/10/2024

Cycle No : 240207


Sample No : 01

Round Open Date : 08/08/2024

Frequency Histogram Your Method

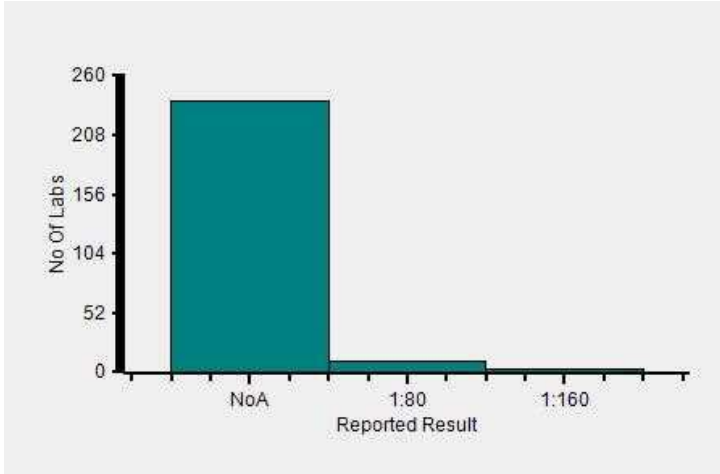

Frequency Histogram Your Analyzer

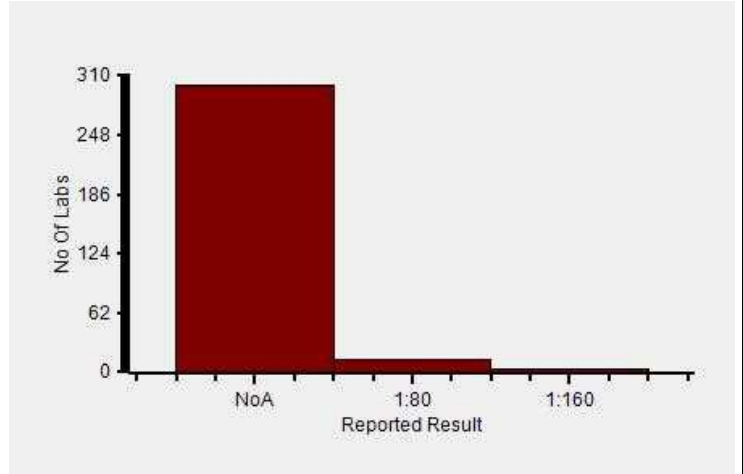

**Reported Results Legends :-**

<b>NoA</b>	: No Agglutination
<b>1:80</b>	: 1:80
<b>1:160</b>	: 1:160
<b>1:320</b>	: 1:320
<b>1:640</b>	: 1:640
<b>&gt;1:640</b>	: >1:640

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- |                       |   |
|-----------------------|---|
| • Two out of two pass | - Acceptable performance                                |
| • One out of two pass | - Review for random error & take action if appropriate  |
| • Both failed         | - Unacceptable performance, Review for systematic error |

b) Reported on 3 samples:

- |                         |   |
|-------------------------|---|
| • All pass              | - Acceptable performance                                |
| • Two out of three pass | - Review for random error & take action if appropriate  |
| • One out of three pass | - Unacceptable performance, Review for systematic error |
| • All failed            | - Unacceptable performance, Review for systematic error |

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**

Unit No. 409-416.

Commercial Building - 1A  
Kohinoor Mall, Kirol Road, Kurla (W),  
Mumbai - 400070

This is a computer generated report hence signature is not required



PC-1022

End of Report

Page 26 of 26